

Алматы (7273)495-231
Ангарск (3955)60-70-56
Архангельск (8182)63-90-72
Астрахань (8512)99-46-04
Барнаул (3852)73-04-60
Белгород (4722)40-23-64
Благовещенск (4162)22-76-07
Брянск (4832)59-03-52
Владивосток (423)249-28-31
Владикавказ (8672)28-90-48
Владимир (4922)49-43-18
Волгоград (844)278-03-48
Вологда (8172)26-41-59
Воронеж (473)204-51-73
Екатеринбург (343)384-55-89

Иваново (4932)77-34-06
Ижевск (3412)26-03-58
Иркутск (395)279-98-46
Казань (843)206-01-48
Калининград (4012)72-03-81
Калуга (4842)92-23-67
Кемерово (3842)65-04-62
Киров (8332)68-02-04
Коломна (4966)23-41-49
Кострома (4942)77-07-48
Краснодар (861)203-40-90
Красноярск (391)204-63-61
Курск (4712)77-13-04
Курган (3522)50-90-47
Липецк (4742)52-20-81

Магнитогорск (3519)55-03-13
Москва (495)268-04-70
Мурманск (8152)59-64-93
Набережные Челны (8552)20-53-41
Нижний Новгород (831)429-08-12
Новокузнецк (3843)20-46-81
Ноябрьск (3496)41-32-12
Новосибирск (383)227-86-73
Омск (3812)21-46-40
Орел (4862)44-53-42
Оренбург (3532)37-68-04
Пенза (8412)22-31-16
Петрозаводск (8142)55-98-37
Псков (8112)59-10-37
Пермь (342)205-81-47

Ростов-на-Дону (863)308-18-15
Рязань (4912)46-61-64
Самара (846)206-03-16
Санкт-Петербург (812)309-46-40
Саратов (845)249-38-78
Севастополь (8692)22-31-93
Саранск (8342)22-96-24
Симферополь (3652)67-13-56
Смоленск (4812)29-41-54
Сочи (862)225-72-31
Ставрополь (8652)20-65-13
Сургут (3462)77-98-35
Сыктывкар (8212)25-95-17
Тамбов (4752)50-40-97
Тверь (4822)63-31-35

Тольятти (8482)63-91-07
Томск (3822)98-41-53
Тула (4872)33-79-87
Тюмень (3452)66-21-18
Ульяновск (8422)24-23-59
Улан-Удэ (3012)59-97-51
Уфа (347)229-48-12
Хабаровск (4212)92-98-04
Чебоксары (8352)28-53-07
Челябинск (351)202-03-61
Череповец (8202)49-02-64
Чита (3022)38-34-83
Якутск (4112)23-90-97
Ярославль (4852)69-52-93

Россия +7(495)268-04-70

Казахстан +7(7172)727-132

Киргизия +996(312)96-26-47

<https://microsensor.nt-rt.ru/> || moj@nt-rt.ru

Высокоточный датчик давления с
аналоговым выходом МРМ483Е.
Технические характеристики.



High Accuracy Analog Output Pressure Transmitter

MPM483E



Applications

- Metallurgy
- Hydrogeology
- Food & Pharmaceutical Industry
- Environmental Control

Features

- High-level electromagnetic compatibility
- Support reverse polarity, instantaneous over-current, over-voltage protection
- LCD and LED digital display
- CE approved

Introduction

MPM483E pressure transmitter is a cost-effective, universal digital pressure transmitter product launched by our company, the product adopts high-stability diffusion silicon pressure core and advanced digital conditioning circuit, combined with mature pressure transmitter design and manufacturing technology, to ensure the accuracy and stability of pressure measurement. The product adopts corrosion-resistant 2088 shell head, which can be applied to relatively severe working conditions; High-brightness LED and backlit LCD display, suitable for places that require on-site inspection; The product as a whole has passed a higher level of electromagnetic compatibility test and can be used for equipment or environments with electromagnetic interference.



Specification

Range	-1bar...0mbar ~ 100mbar...1000bar
Over pressure	$\leq 2 \times \text{FS}$ or 1100bar (whichever is less)
Pressure Type	gauge, absolute, sealed gauge
Accuracy	see the "Accuracy"
Long-term Stability	$\pm 0.3\% \text{FS/year}$
Operation Temperature	-30°C ~ 80°C (General type)
	-20°C ~ 60°C (with LCD display)
	-30°C ~ 70°C (with LED display)
Storage Temperature	-40°C ~ 120°C
Vibration	10g, 55Hz ~ 2000Hz
Impact	100g, 11ms
Protection Degree	IP65
Weight	$\leq 375\text{g}$

Accuracy

Pressure Type	Range	Accuracy
Gauge (G)	0mbar ~ 100mbar < X < 200mbar	±1.0%FS
	200mbar ≤ X ≤ 1bar	±0.5%FS
	1bar < X ≤ 35bar	±0.25%FS
		±0.5%FS
	-1bar ~ -350mbar < X ≤ 2bar	±1.0%FS
	-1bar ~ -350mbar < X < 2bar ~ 35bar	±0.5%FS
Absolute (A)	0mbar ~ 700mbar < X ≤ 1bar	±1.0%FS
	1bar < X ≤ 10bar	±0.5%FS
	10bar < X ≤ 1000bar	±0.25%FS
		±0.5%FS
Sealed Gauge (S)	35bar < X ≤ 1000bar	±0.25%FS
		±0.5%FS

Test Standard: GB/T 17614.1-2015/IEC60770-1:2010
 Ambient Temperature: 20°C ±5°C
 Relative Humidity: 45% ~ 75%

Thermal Error

Thermal Error-Offset	±0.05%FS/°C (<200mbar)
	±0.03%FS/°C (200mbar ≤ X ≤ 1bar)
	±0.02%FS/°C (>1bar)
Thermal Error-Span	±0.05%FS/°C (<200mbar)
	±0.03%FS/°C (200mbar ≤ X ≤ 1bar)
	±0.02%FS/°C (>1bar)

Output Signal

Output Signal	Supply Voltage	Connection	Load Resistance
4mA~20mA DC(E)	11V ~ 28V DC	2-wire	≤(U-11)/0.02(Ω)
0V~5V DC(J)	15V ~ 28V DC	3-wire	≥10kΩ
1V~5V DC(F)			
0V~10V DC(V)			

Electromagnetic Compatibility



S.N.	Test Item	Standard	Test Condition	Performance Level
①	Electrostatic Discharge Immunity	EN IEC 61000-6-2:2019&IEC 61000-4-2:2008	±4kV (touch) ±8kV (air)	B
②	RF Radiated Immunity	EN IEC 61000-6-2:2019&IEC 61000-4-3:2020	80MHz~1000MHz 10V/m 1400MHz~6000MHz 3V/m	A
③	Electrical Fast Pulse Immunity	EN IEC 61000-6-2:2019&IEC 61000-4-4:2012	1kV	B
④	Surge Immunity	EN IEC 61000-6-2:2019&IEC 61000-4-5:2014	line-line 0.5kV line-ground 1kV	B
⑤	Conducted RF Immunity	EN IEC 61000-6-2:2019&IEC 61000-4-2:2013	0.15MHz~80MHz	A
⑥	Power Frequency Magnetic Field	EN IEC 61000-6-2:2019&IEC 61000-4-8:2009	30A/m	A

Performance Level A: normal performance within limits specified by the manufacturer, contractor or purchaser;


Performance Level B: temporary loss or reduction in function or performance, but self-recovery after the disturbance ceases without operator intervention

Outline Dimension

unit: mm

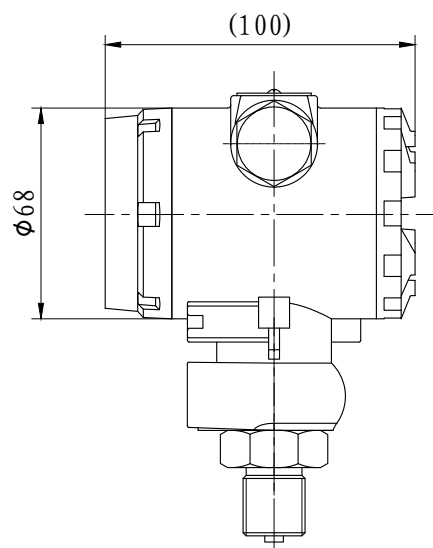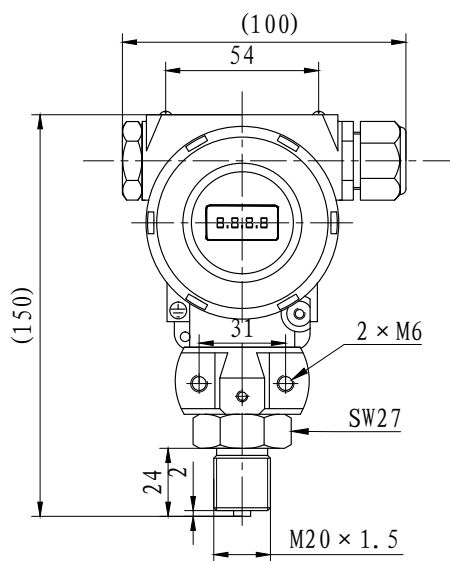

Electrical Connection

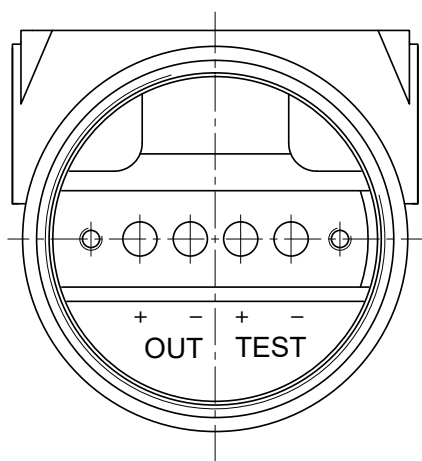

Current Type		Voltage Type	
Terminal	Signal	Terminal	Signal
OUT+	V+	OUT+	V+
OUT-	IO	OUT-	OUT
null	null	TEST-	GND

Materials

Wetted Parts

Isolated Diaphragm: Stainless Steel 316L/Tantalum

Pressure Port: Stainless Steel 304/ Stainless Steel 316L/Hastelloy C


Non-wetted Parts

Housing: Aluminum Alloy


Process Connection

unit: mm


M20×1.5 Male, End Face Seal (C1)




NPT1/4 Male (C6)

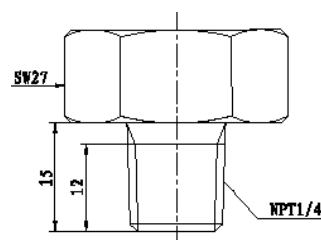


G1/4 Male, End Face Seal (C2)




M20×1.5 or G1/2 Flush Diaphragm (PC1/PC3)




G1/2 Male, End Face Seal (C3)




DN25 Tri-clamp (PD1)

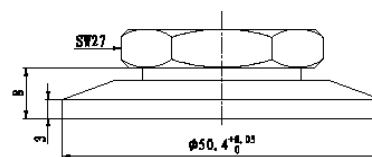

M20×1.5 Male, Waterline Seal (C5)



DN25 Tri-clamp with Heat Sink (PD1s)

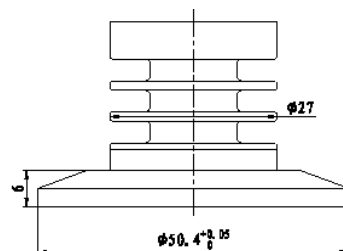

Order Guide

MPM483E	Pressure Transmitter									
	Range	Measured range: -1bar...0mbar ~ 100mbar...1000bar								
	[0 ~ X]mbar or bar	X: Actual Measured Range								
		Code	Pressure Type							
		G	gauge							
		A	absolute							
		S	sealed gauge							
		Code	Accuracy ^①							
		A1	±0.25% FS							
		A2	±0.5% FS							
		A3	±1% FS							
		Code	Output Signal							
		E	4mA~20mA DC							
		J	0V~5V DC							
		F	1V~5V DC							
		V	0V~10V DC							
		Code	Material							
			Isolated Diaphragm	Pressure Port		Housing				
		22	S.S. 316L	S.S. 304		Aluminum Alloy				
		24	S.S. 316L	S.S. 316L						
		25	Tantalum	S.S. 304						
		35	Tantalum	Hastelloy C						
		Code	Process Connection							
		C1	M20×1.5 male, end face seal							
		C2	G1/4 male, end face seal							
		C3	G1/2 male, end face seal							
		C5	M20×1.5 male, waterline seal							
		C6	NPT1/4 male							
		PC1	M20×1.5 flush diaphragm		0 mbar ~ 200mbar...350bar					
		PC3	G1/2 flush diaphragm							
		PD1	DN25 tri-clamp		0 mbar ~ 350mbar...35bar					
		PD1s	DN25 tri-clamp with the heat sink							
		Code	Accessories							
		Null	Null							
		M6	4 -bit LED Digital Display (for 4mA ~ 20mA DC only)							
		M7	4 -bit LCD Digital Display (for 4mA ~ 20mA DC only)							
MPM483E	[0 ~10]bar	G	A1	E	22	C1	M6	Complete Part Number		

Order Notes

1. " ① " in Order Guide table indicates the product accuracy parameters, see "Accuracy" on page 2 for details.
2. Please note the power supply should be $\geq 16V$ DC when ordering a transmitter with M6 or M7 display.
3. For the product measurement certificate or other special requirements, please contact with us and note in the order.

Алматы (7273)495-231
 Ангартк (3955)60-70-56
 Архангельск (8182)63-90-72
 Астрахань (8512)99-46-04
 Барнаул (3852)73-04-60
 Белгород (4722)40-23-64
 Благовещенск (4162)22-76-07
 Брянск (4832)59-03-52
 Владивосток (423)249-28-31
 Владикавказ (8672)28-90-48
 Владимир (4922)49-43-18
 Волгоград (844)278-03-48
 Вологда (8172)26-41-59
 Воронеж (473)204-51-73
 Екатеринбург (343)384-55-89

Иваново (4932)77-34-06
 Ижевск (3412)26-03-58
 Иркутск (395)279-98-46
 Казань (843)206-01-48
 Калининград (4012)72-03-81
 Калуга (4842)92-23-67
 Кемерово (3842)65-04-62
 Киров (8332)68-02-04
 Коломна (4966)23-41-49
 Кострома (4942)77-07-48
 Краснодар (861)203-40-90
 Красноярск (391)204-63-61
 Курск (4712)77-13-04
 Курган (3522)50-90-47
 Липецк (4742)52-20-81

Магнитогорск (3519)55-03-13
 Москва (495)268-04-70
 Мурманск (8152)59-64-93
 Набережные Челны (8552)20-53-41
 Нижний Новгород (831)429-08-12
 Новокузнецк (3843)20-46-81
 Ноябрьск (3496)41-32-12
 Новосибирск (383)227-86-73
 Омск (3812)21-46-40
 Орел (4862)44-53-42
 Оренбург (3532)37-68-04
 Пенза (8412)22-31-16
 Петрозаводск (8142)55-98-37
 Псков (8112)59-10-37
 Пермь (342)205-81-47

Ростов-на-Дону (863)308-18-15
 Рязань (4912)46-61-64
 Самара (846)206-03-16
 Санкт-Петербург (812)309-46-40
 Саратов (845)249-38-78
 Севастополь (8692)22-31-93
 Саранск (8342)22-96-24
 Симферополь (3652)67-13-56
 Смоленск (4812)29-41-54
 Сочи (862)225-72-31
 Ставрополь (8652)20-65-13
 Сургут (3462)77-98-35
 Сыктывкар (8212)25-95-17
 Тамбов (4752)50-40-97
 Тверь (4822)63-31-35

Тольятти (8482)63-91-07
 Томск (3822)98-41-53
 Тула (4872)33-79-87
 Тюмень (3452)66-21-18
 Ульяновск (8422)24-23-59
 Улан-Удэ (3012)59-97-51
 Уфа (347)229-48-12
 Хабаровск (4212)92-98-04
 Чебоксары (8352)28-53-07
 Челябинск (351)202-03-61
 Череповец (8202)49-02-64
 Чита (3022)38-34-83
 Якутск (4112)23-90-97
 Ярославль (4852)69-52-93

Россия +7(495)268-04-70

Казахстан +7(7172)727-132

Киргизия +996(312)96-26-47

<https://microsensor.nt-rt.ru/> || moj@nt-rt.ru