

Алматы (7273)495-231
Ангарск (3955)60-70-56
Архангельск (8182)63-90-72
Астрахань (8512)99-46-04
Барнаул (3852)73-04-60
Белгород (4722)40-23-64
Благовещенск (4162)22-76-07
Брянск (4832)59-03-52
Владивосток (423)249-28-31
Владикавказ (8672)28-90-48
Владимир (4922)49-43-18
Волгоград (844)278-03-48
Вологда (8172)26-41-59
Воронеж (473)204-51-73
Екатеринбург (343)384-55-89

Иваново (4932)77-34-06
Ижевск (3412)26-03-58
Иркутск (395)279-98-46
Казань (843)206-01-48
Калининград (4012)72-03-81
Калуга (4842)92-23-67
Кемерово (3842)65-04-62
Киров (8332)68-02-04
Коломна (4966)23-41-49
Кострома (4942)77-07-48
Краснодар (861)203-40-90
Красноярск (391)204-63-61
Курск (4712)77-13-04
Курган (3522)50-90-47
Липецк (4742)52-20-81

Магнитогорск (3519)55-03-13
Москва (495)268-04-70
Мурманск (8152)59-64-93
Набережные Челны (8552)20-53-41
Нижний Новгород (831)429-08-12
Новокузнецк (3843)20-46-81
Ноябрьск (3496)41-32-12
Новосибирск (383)227-86-73
Омск (3812)21-46-40
Орел (4862)44-53-42
Оренбург (3532)37-68-04
Пенза (8412)22-31-16
Петрозаводск (8142)55-98-37
Псков (8112)59-10-37
Пермь (342)205-81-47

Ростов-на-Дону (863)308-18-15
Рязань (4912)46-61-64
Самара (846)206-03-16
Санкт-Петербург (812)309-46-40
Саратов (845)249-38-78
Севастополь (8692)22-31-93
Саранск (8342)22-96-24
Симферополь (3652)67-13-56
Смоленск (4812)29-41-54
Сочи (862)225-72-31
Ставрополь (8652)20-65-13
Сургут (3462)77-98-35
Сыктывкар (8212)25-95-17
Тамбов (4752)50-40-97
Тверь (4822)63-31-35

Тольятти (8482)63-91-07
Томск (3822)98-41-53
Тула (4872)33-79-87
Тюмень (3452)66-21-18
Ульяновск (8422)24-23-59
Улан-Удэ (3012)59-97-51
Уфа (347)229-48-12
Хабаровск (4212)92-98-04
Чебоксары (8352)28-53-07
Челябинск (351)202-03-61
Череповец (8202)49-02-64
Чита (3022)38-34-83
Якутск (4112)23-90-97
Ярославль (4852)69-52-93

Россия +7(495)268-04-70

Казахстан +7(7172)727-132

Киргизия +996(312)96-26-47

<https://microsensor.nt-rt.ru/> || moj@nt-rt.ru

Интеллектуальный дифференциальный датчик давления с дистанционным мембранным уплотнением MDM7000-LP. Технические характеристики.



Range

Nominal range	Minimum range	Lower (LRL)	Upper (URL)
0.4bar	0.1bar	-0.4bar	0.4bar
2.5bar	0.25bar	-2.5bar	2.5bar

LRV/URV setting: the lower limit value (LRV) and upper limit value (URV) are achieved between the upper and lower limits. If $|URV| \geq LRV$, $|URV|$ must be larger than the minimum pressure; if $|URV| \leq |LRV|$, $|LRV|$ must be larger than the minimum pressure.

It is recommended to choose a range ratio with the minimum possible value.

Accuracy

1 Stated reference accuracy include best fit straight line(BFSL), hysteresis, and repeatability as per the standard and reference test conditions. Calibration temperature: 20°C ±5°C, based on Zero value.

2 Total performance is based on combined errors of indoor temperature accuracy, ambient temperature effects and static pressure effects, calculated by the following formula: Total performance = $\pm\sqrt{(E1)^2 + (E2)^2 + (E3)^2}$;

E1=Indoor temperature accuracy E2=Ambient temperature effects E3=Static pressure effects

Linear output accuracy	TD≤5	±0.25% +Diaphragm seal system effects	0.4bar, 2.5bar
	TD > 5	±(0.025%×0.045TD) % +Diaphragm seal system effects	

Square root output accuracy is 1.5 times linear output accuracy.

Note: TD(Turn down) represents the range ratio, TD= Maximum range / Current range
[Maximum range = URL (range starts with 0, same as factory calibration range); Current range = SPAN (equivalent to |URV-LRV|)].

Specifications

Accuracy	±0.2% URL + Diaphragm seal system effects
Range	0.4bar~2.5bar, see the specifications for details
Long-term stability	±0.2% Span/5 years
Ambient temperature effects	The total effect per 10°C in the range of -20°C ~80°C: (0.375+0.125TD)%/10°C of SPAN
Voltage effects	When the power supply voltage changes within 10.5V/16.5V ~55V DC, its zero point and range change should not exceed ±0.005% URL/V
Mounting position effects	The installation of the transmitter may produce a zero point error, which can be corrected by PV (primary value) =0 reset without any effect on the range.
Vibration effects	< 0.1% SPAN as per GB/T18271.3/IEC61298-3
Output signal	4mA~20mA DC, HART
IP rating	IP67
Weight	About:6.5kg(body)

EMC Effects

SN	Test items	Basic Standards	Test Conditions	Performance Level
1	Radiated interference (case)	GB/T 9254.1/CISPR 32	30MHz~1000MHz	Qualified
2	Conducted interference (DC power port)	GB/T 9254.1/CISPR 32	0.15MHz~30MHz	Qualified
3	Electrostatic discharge (ESD) immunity test	GB/T 17626.2/IEC61000-4-2	4kV(Contact), 6kV(Air)	B
4	Radiated, radio-frequency, electromagnetic field immunity test	GB/T 17626.3/IEC61000-4-3	10V/m (80MHz~1GHz)	A
5	Power frequency magnetic field immunity test	GB/T 17626.8/IEC61000-4-8	30A/m	A
6	Electrical fast transient / burst immunity test	GB/T 17626.4/IEC61000-4-4	2kV(5/50ns,100kHz)	B
7	Surge immunity test	GB/T 17626.5/IEC61000-4-5	500V(line to line) 1kV (line to ground) (1.2/50μs)	B
8	Immunity to conducted disturbances induced by radio frequency fields	GB/T 17626.6/IEC61000-4-6	3V(150kHz~80MHz)	A

Note: At performance level A, the performance is normal within the limits of the technical specifications.

At performance level B, functions or performance are temporarily reduced or lost, but can be restored by themselves, and the actual operating conditions, storage and data remain unchanged.

|| Environmental Conditions ||

Items	Conditions
Operating temperature	Without LCD display: -40°C ~85°C ; with LCD display: -20°C ~70°C
Storage temperature	Without LCD display: -40°C ~100°C ; with LCD display: -40°C ~85°C
Operating humidity	5%RH~100%RH@40°C


|| Diaphragm Operating Temperature ||

Filling oil type ^①	Code	Medium temperature	Diaphragm ambient temperature
Normal temperature silicone oil	S	-40°C~ 205°C	-40°C~ 85°C
Inert filling oil	D	-45°C~ 160°C	-40°C~ 85°C
High temperature silicone oil	H	0°C~ 315°C	0°C~ 85°C

Note:^① This item is related to the type of silicone oil filled and the o-ring; the temperature range of non-silicone oil is limited to the lowest material temperature range in the system. For short-pipe explosion-proof products, users need to ensure that the surface temperature of the shell is not higher than 80° C. If uncertain, the medium temperature must be ensured not to be higher than the T6/ T80° C temperature group.

|| Power Supply and Load Requirements ||

Items	Conditions
Power supply voltage	HART communication protocol: 16.5V~55V DC ^①
	Intrinsically safe HART communication protocol: 18.5V~28V DC
Load resistance	0Ω~2119Ω ^② for operation mode; 250Ω~600Ω for HART communication
Transmission distance	<1000m
Power consumption	
4mA~20mA	≤500mW@24V DC, 20.8mA

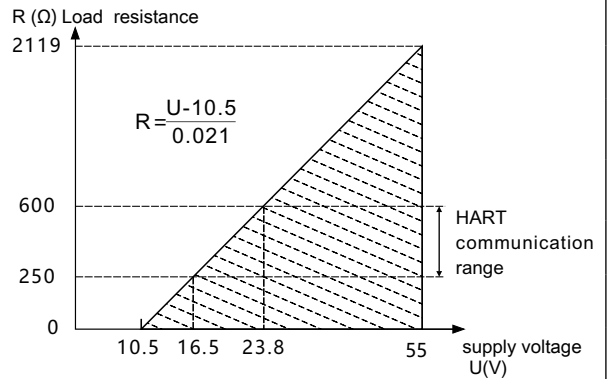

Note:^① Non intrinsically safe power supply voltage can be selected as 10.5V. Please consult engineers for details.

^② 2119Ω= (55V-10.5V) /21mA

|| Time Index ||

Damping time constant: equals to the combined damping time of electronic components and sensor module
Electronic components damping time: 0s~100s configurable
Sensor module damping time(sensor isolated diaphragm and filled silicone oil):≤ 0.2s (Note: This item is related to the sensor type and whether there is a diaphragm component.)
Turn-on time: ≤6s
Factory reset time: ≤31s

|| Hazardous Area ||


Hazardous area ^①	PCEC	Ex db IIC T6 Gb Ex ia IIC T4 Ga
	NEPSI	Ex tb III C T85°C Db
	ATEX	Ex ia IIC T4 Ga II 2G Ex db IIC T6 Gb II 2D Ex tb IIIC T80°C Db
	IECEX	Ex ia IIC T4 Ga Ex db IIC T6 Gb Ex tb IIIC T80°C Db
	CSA	Class I, Division 1, Group A, B, C and D T6 Class II, Division 1 Group E, F and G T80°C Class III Ex db IIC T6 Gb Class I, Zone 1, AEx db IIC T6 Gb Ex tb IIIC T80°C Db Zone 21, AEx tb IIIC T80°C Db
Note: ^① Please consult engineers for details.		

Dimensions


Unit: mm

Note: The gland head is sent as an accessory with the product when it leaves the factory, and it is to be installed by the user.

Remote Fixed Flange + Remote Fixed Flange With Display (Same as Without Display)

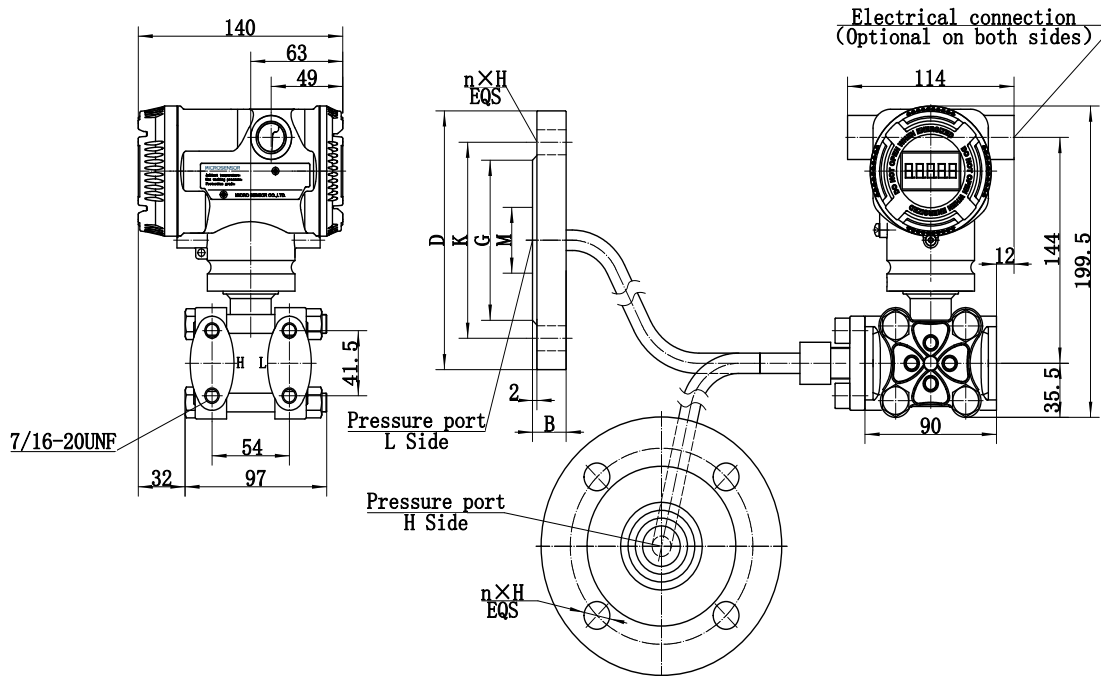


Remote Fixed Flange Insertion Sleeve + Remote Fixed Flange With Display (Same as Without Display)

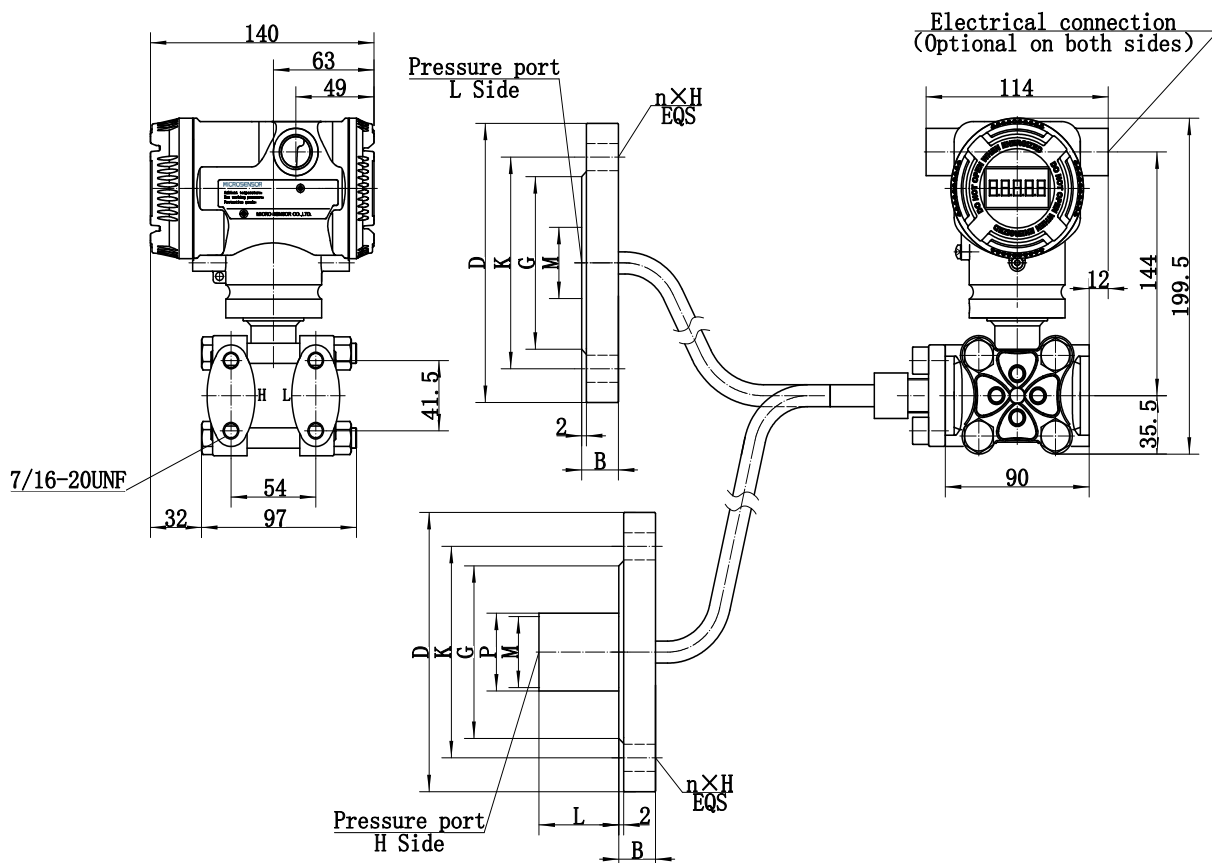


Remote Fixed Flange Insertion Sleeve + Remote Fixed Flange Insertion Sleeve With Display

(Same as Without Display)

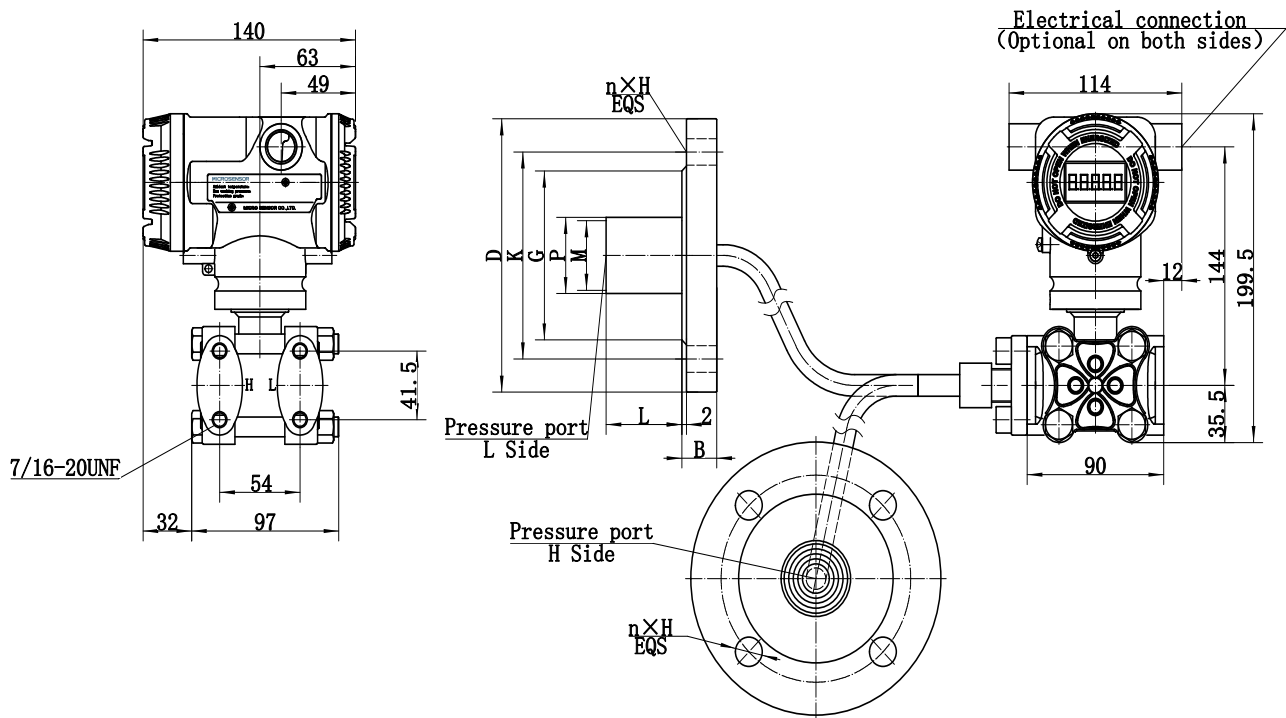


Side Mounted Movable Flange + Remote Fixed Flange With Display


(Same as Without Display)

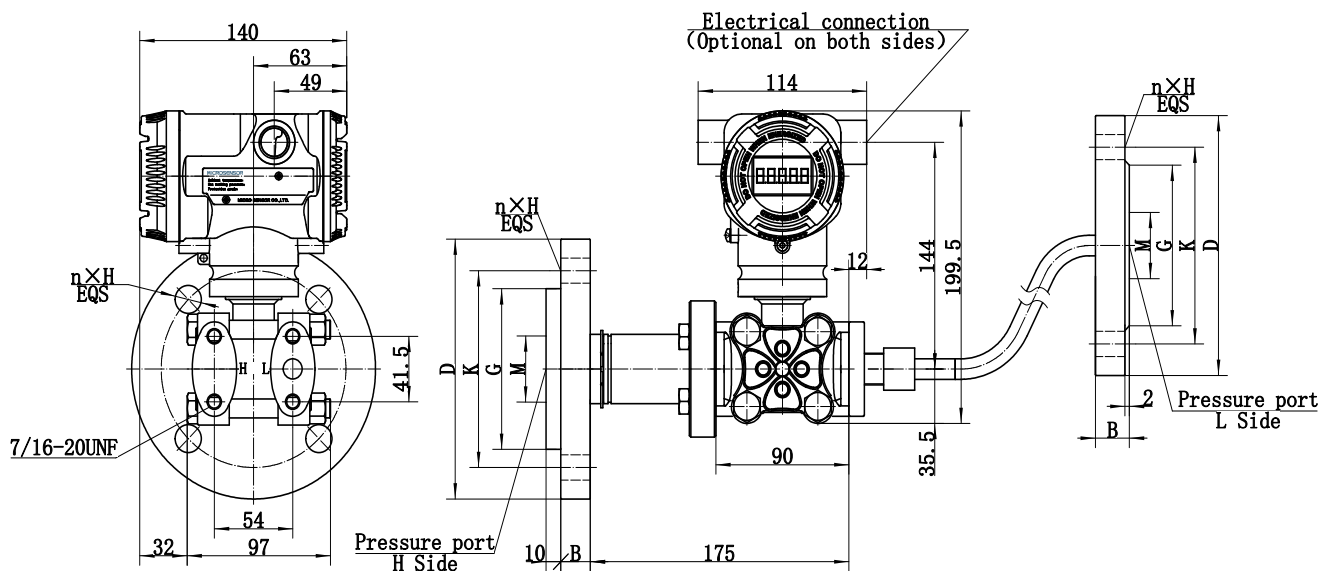


(Same as Without Display)

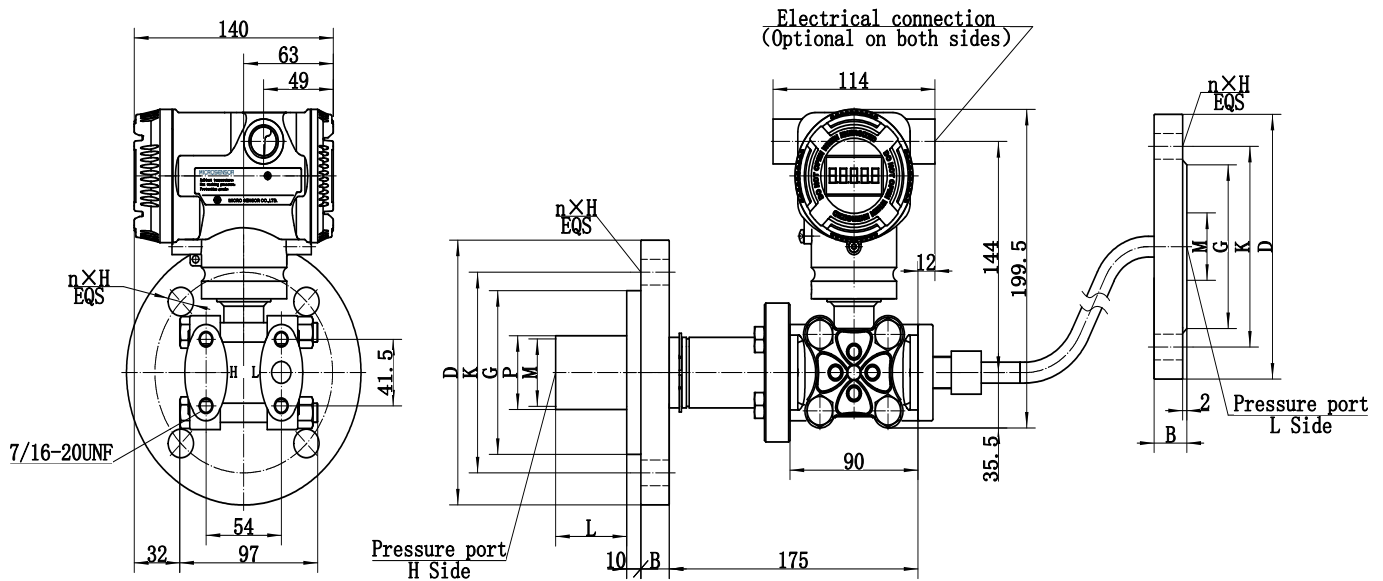

(Same as Without Display)

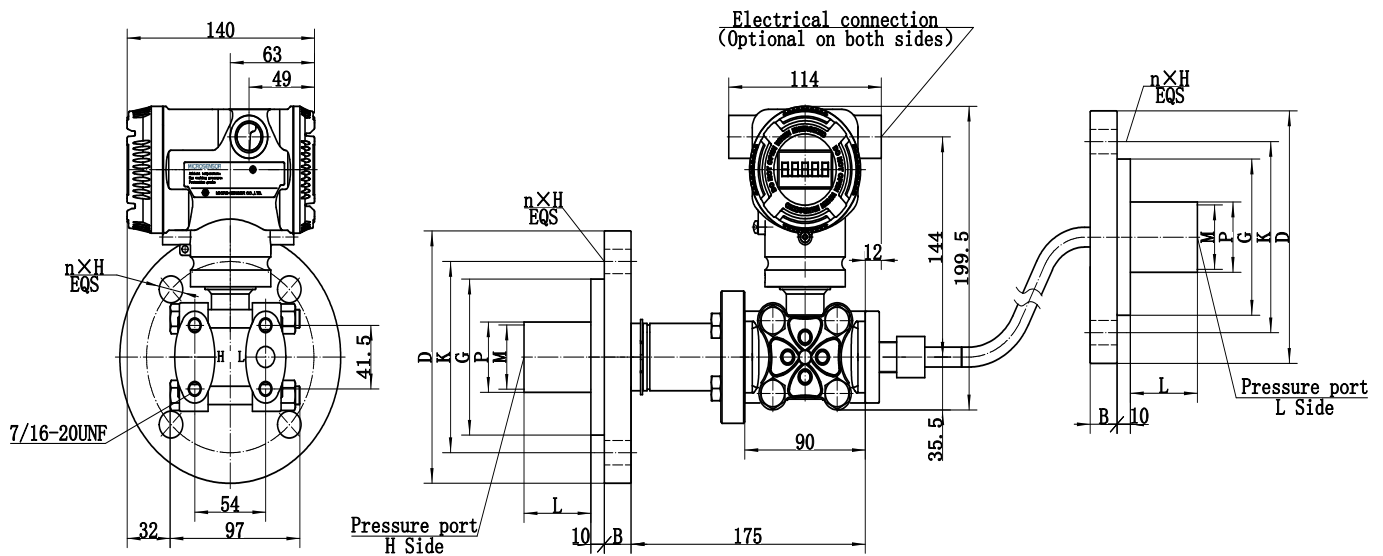


Process Connection

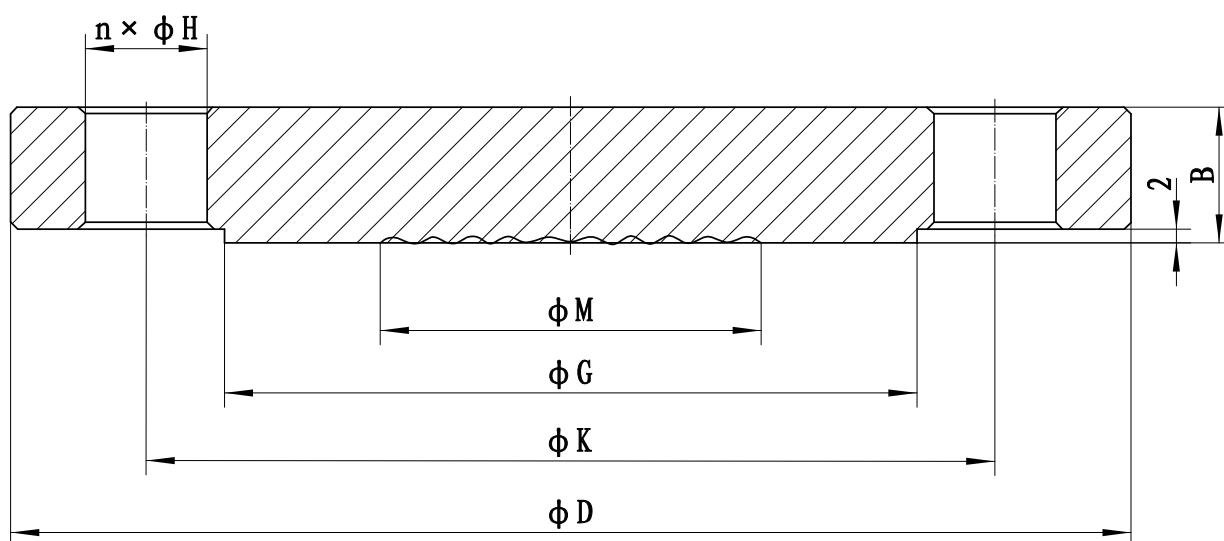

Standard	Specification	Outer diameter (ϕD)	Thickness (B)	Hole circumference (ϕK)
HG/T20592-2009	DN50PN10	165	20	125
HG/T20592-2009	DN80PN10	200	20	160
HG/T20592-2009	DN100PN10	220	20	180
RF diameter (ϕG)	Hole diameter (ϕH)	Quantity (n)	Corrugation diameter (ϕM)	
102	18	4	56	
138	18	8	56	
158	18	8	56	

Process Connection

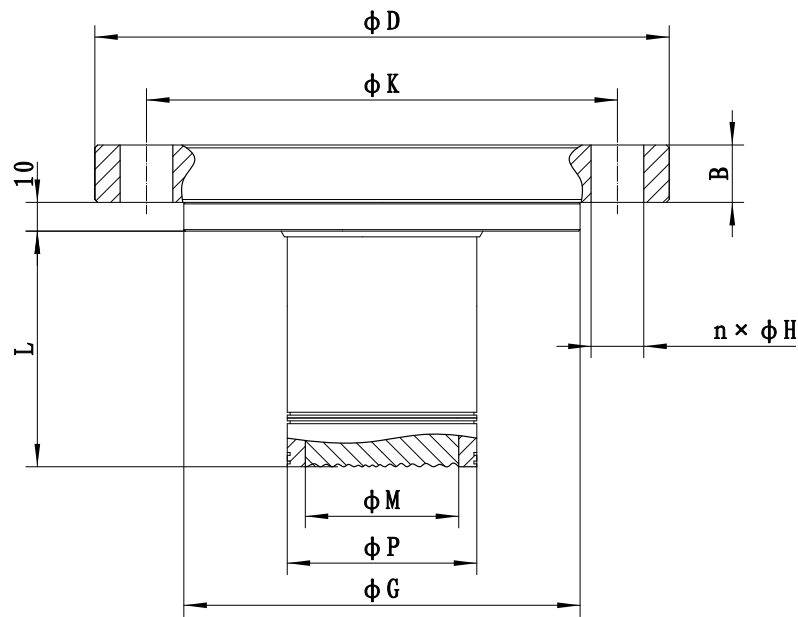

Standard	Specification	Outer diameter(ϕD)	Thickness(B)	RF diameter(ϕG)	Hole circumference (ϕK)
HG/T20592-2009	DN80PN10	200	20	138	160
HG/T20592-2009	DN80PN10	200	20	138	160
HG/T20592-2009	DN80PN10	200	20	138	160
HG/T20592-2009	DN50PN10	165	20	102	125
HG/T20592-2009	DN50PN10	165	20	102	125
HG/T20592-2009	DN50PN10	165	20	102	125
Quantity (n)	Hole diameter (ϕH)	Insertion sleeve diameter (ϕP)	Insertion sleeve length (L)	Corrugation diameter (ϕM)	
8	18	66	50	42	
8	18	66	100	42	
8	18	66	150	42	
4	18	46	150	42	
4	18	46	50	42	
4	18	46	100	42	

|| Order Guide ||

MDM7000-LP — □□□□□ — □ — **HF** — □□□□□ — **LF** — □□□□□
Body **Remote Flange+Remote Flange Diaphragm**

Item	Code	Description				
MDM7000-LP	—	Monocrystalline Silicon Differential Pressure Transmitter with Diaphragm Seals (Remote Fixed Flange + Remote Fixed Flange)				
Application of hazardous area						
	1	China, Flameproof certificate, No.CE23.6650 Ex db IIC T6 Gb, GB/T3836.1-2021, GB/T3836.2-2021				
	2	China, Intrinsically safe certificate, No.CE23.7688X Ex ia IIC T4 Ga, GB/T3836.1-2021, GB/T3836.4-2021				
	3	China, Dust explosion-proof certificate, GYB24.1215X Ex tb III C T85°C Db, GB/T3836.1-2021, GB/T 3836.31-2021				
	4	China, Flameproof certificate, Intrinsically safe certificate				
	A	CSA, Flameproof certificate				
	B	CSA, Intrinsically safe certificate				
	C	CSA, Flameproof certificate, Intrinsically safe certificate				
	E	ATEX, Flameproof certificate				
	F	ATEX, Intrinsically safe certificate				
	G	ATEX, Flameproof certificate, Intrinsically safe certificate				
	J	IECEx, Flameproof certificate	 			
	K	IECEx, Intrinsically safe certificate				
	L	IECEx, Flameproof certificate, Intrinsically safe certificate				
	0	Non-hazardous area				
	T	Other certificate				
Output signal	H	4mA~20mA DC, HART				
Case	S	Stainless steel case with two outlet ports (F) M20×1.5				
	U	Stainless steel case with two outlet ports (F) 1/2NPT				
	P	Aluminum alloy case with two outlet ports (F) M20×1.5				
	N	Aluminum alloy case with two outlet ports (F) 1/2NPT				
Note: Please pay attention to the item of lithium battery (Code: LD)						
Waterproof/explosion-proof connector						
		Specification	Material	Applicable wire diameter	IP rating	
	1	M20×1.5 waterproof connector, with plug	PVC	6mm~8mm	IP67	
	2	Non-flameproof adapter (F) M20×1.5, with plug	316 SS	6mm~8mm	IP67	
	3	Flameproof adapter (F) 1/2NPT, with plug	316 SS	6mm~8mm	IP67	
	4	Flameproof adapter (F) M20×1.5, with plug	316 SS	6mm~8mm	IP67	
	5	Flameproof adapter (F) G1/2, with plug	316 SS	6mm~8mm	IP67	
Note: Flameproof configuration is applicable to PCEC/ATEX/IECEx standards. Flameproof adapter with CCC certificate. Please contact the engineer if double sealing is required.						
Display	N	Without LCD display				
	L	Display module, -20°C ~70°C				
Sensor module range						
		Nominal range	Minimum range	Lower (LRL)	Upper (URL)	
	2	0.4bar	0.1bar	-0.4bar	0.4bar	
	3	2.5bar	0.25bar	-2.5bar	2.5bar	
Flange block fastener	6	Bolts, nuts, and other components, 316 SS				
—						

Diaphragm connection position	H	Differential pressure transmitter high pressure side		
Diaphragm seal system code	F	Remote fixed flange		
Flange standard	2	HG/T-20592		
	1	EN1092-1		
	5	HG/T-20615		
	6	ANSI/ASME B16.5		
Flange diameter	Applicable standard			
	B	DN50	HG/T-20592, EN1092-1	
	C	DN80	HG/T-20592, EN1092-1	
	D	DN100	HG/T-20592, EN1092-1	
	2	2inch	HG/T-20615, ANSI/ASME B16.5	
	3	3inch	HG/T-20615, ANSI/ASME B16.5	
	4	4inch	HG/T-20615, ANSI/ASME B16.5	
Pressure class	Applicable standard			
	Applicable flange diameter			
	1	PN10/PN16	HG/T-20592, EN1092-1	DN50, DN80, DN100
	2	PN25/PN40	HG/T-20592, EN1092-1	DN50, DN80, DN100
	3	PN63	HG/T-20592, EN1092-1	DN50, DN80
	4	PN100	HG/T-20592, EN1092-1	DN50, DN80
	A	Class 150	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	B	Class 300	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
C	Class 600	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch	
Note: The maximum static pressure or overload depends on the flange pressure class				
Flange material	6	316 SS		
Flange sealing surface	1	RF Raised surface		
	A	FM Concave surface		
	B	M Convex surface		
	C	RJ Annular connection surface		
Note: For details about FM concave, M convex, RJ annular connection surface, please consult the engineer				
Wetted parts material	Please see the material list of wetted parts for details			
		Blind	Measuring diaphragm	
	6A	316 SS	316L	
	6B	316 SS	Hastelloy C-276	
	6C	316 SS	Tantalum	
	6D	316 SS	Titanium	
	6E	316 SS	Monel	
Capillary connection location	K	Rear connection		
Capillary type	U	3.5mm OD (or 1/8 inch), armored 316L SS, PVC gray sheath		
	L	3.5mm OD (or 1/8 inch), armored 316L SS, stainless steel bellows sheath		

Capillary length		Applicable flange diameter		
		DN50/2inch	DN80/3inch	DN100/4inch
1	1m			
2	2m			
3	3m			
4	4m			
5	5m			
6	6m	×		
7	7m	×		
8	8m	×		
9	9m	×		
A	10m	×		

Note: "×" means unavailable; the part beyond the length will be selected according to the next level of meters.

High pressure side fill oil	S	Normal temperature silicone oil (Medium temperature : -40°C ~205°C , diaphragm ambient environment: -40°C ~85°C)		
	D	Inert oil (Medium temperature: -45°C ~160°C ,diaphragm ambient environment:-40°C ~85°C)		
	H	High temperature silicone oil (Medium temperature: 0°C ~315°C , diaphragm ambient environment: 0°C ~85°C)		
Diaphragm connection position	L	Differential pressure transmitter low pressure side		
Diaphragm seal system code	F	Remote fixed flange		

Flange standard	2	HG/T-20592		
	1	EN1092-1		
	5	HG/T-20615		
	6	ANSI/ASME B16.5		

Flange diameter		Applicable standard		
B	DN50	HG/T-20592, EN1092-1		
C	DN80	HG/T-20592, EN1092-1		
D	DN100	HG/T-20592, EN1092-1		
2	2inch	HG/T-20615, ANSI/ASME B16.5		
3	3inch	HG/T-20615vANSI/ASME B16.5		
4	4inch	HG/T-20615, ANSI/ASME B16.5		

Pressure class		Applicable standard		Applicable flange diameter	
1	PN10/PN16	HG/T-20592, EN1092-1		DN50, DN80, DN100	
2	PN25/PN40	HG/T-20592, EN1092-1		DN50, DN80, DN100	
3	PN63	HG/T-20592, EN1092-1		DN50, DN80	
4	PN100	HG/T-20592, EN1092-1		DN50, DN80	
A	Class 150	HG/T-20615, ANSI/ASME B16.5		2inch, 3inch, 4inch	
B	Class 300	HG/T-20615, ANSI/ASME B16.5		2inch, 3inch, 4inch	
C	Class 600	HG/T-20615, ANSI/ASME B16.5		2inch, 3inch	

Note: The maximum static pressure or overload depends on the flange pressure class

Flange material	6	316 SS		
-----------------	---	--------	--	--

Blind sealing surface	1	RF Raised surface
	A	FM Concave surface
	B	M Convex surface
	C	RJ Annular connection surface

Note: For details about FM concave, M convex, RJ annular connection surface, please consult the engineer

Wetted parts material	Please see the material list of wetted parts for details	
	Blind	Measuring diaphragm
	6A	316 SS 316L
	6B	316 SS Hastelloy C-276
	6C	316 SS Tantalum
	6D	316 SS Titanium
	6E	316 SS Monel

Capillary connection location	K	Rear connection
-------------------------------	---	-----------------

Capillary type	U	3.5mm OD (or 1/8 inch), armored 316L SS, PVC gray sheath
	L	3.5mm OD (or 1/8 inch), armored 316L SS, stainless steel bellows sheath

Capillary length	Applicable flange diameter		
		DN50/2inch	DN80/3inch
			DN100/4inch
1	1m		
2	2m		
3	3m		
4	4m		
5	5m		
6	6m	x	
7	7m	x	
8	8m	x	
9	9m	x	
A	10m	x	

Note: "x" means unavailable; the part beyond the length will be selected according to the next level of meters.

Low pressure side fill oil	S	Normal temperature silicone oil (Medium temperature : -40°C ~205°C , diaphragm ambient environment: -40°C ~85°C)
	D	Inert oil (Medium temperature: -45°C ~160°C ,diaphragm ambient environment:-40°C ~85°C)
	H	High temperature silicone oil (Medium temperature: 0°C ~315°C , diaphragm ambient environment: 0°C ~85°C)

Factory calibration range	CAL	Provides Micro Sensor standard verification report according to the range, and the default linear output Contract specifies: LRL - URL, display unit*
---------------------------	-----	---

Options	Description (Detailed specifications as following, multiple options or null)	
---------	--	--

High vacuum high temperature	/V	High vacuum and high temperature process diaphragm (if this option is selected, the accuracy will be affected and can only up to 0.2%)
------------------------------	----	--

Mounting bracket	/G1	Bent bracket, 316 SS
------------------	-----	----------------------

Verification report	/Q1	Provide the Micro Sensor verification data according to user requirements Contract specifies: LRL - URL, display unit*
---------------------	-----	--

Note: Standard format follows the Micro Sensor's specifications. Select this option and provide the template if the customer specifies a format

Damping time setting	/ST	Adjustable range 0~100s, default 0s Contract specifies: Damping time*
----------------------	-----	---

Fault alarm setting	/WH	High alarm current value, 20.8mA
	/WL	Low alarm current value, 3.8mA, default
	/WS	Other saturation current values, specified within the range of 3.6mA~3.8mA or 20mA~22mA Contract specifies: saturation current values *
Product certificate	/QE	Standard format follows the Micro Sensor's specifications. Select this option and provide the template if the customer specifies a format
Identification plate	/PT	Product is shipped with an identification plate Contract specifies: Complete model of Micro Sensor valve manifold*
Leakage test report	/QD4	PN10/PN16 (class150) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD5	PN25/PN40 (class300) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD6	PN63, Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD7	PN100 (class600) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report

Note: The test pressure is the same as the flange pressure class

HART configuration	/H5	HART5 configuration
Diaphragm with gold plated	/J3	Single diaphragm on high pressure side (5μ)
	/J4	Double diaphragms on high and low pressure sides (5μ)
Diaphragm spraying	/T1	High pressure side single flange
	/T2	High-low pressure side double flanges
Diaphragm sticking	/PFA	The diaphragm is stuck with PFA film, applicable to non-vacuum situations (pressure ≥ 0)
Oil-free treatment	/CL1	Degreasing and cleaning treatment of the wetted parts

Note: Please check the fill oil. Determine whether the inert filling oil is required (code: D).

Certificates	/CS1	CCS, China Classification Society, TJ23PTB00014
	/CS2	DNV, Det Norske Veritas
	/CS3	BV, Bureau Veritas
	/CS4	ABS, American Bureau of Shipping
	/CS5	LR, Lloyd's Register of Shipping
	/CS6	KR, Korean Register of Shipping
	/CS7	NK, Nippon Kaiji Kyokai
	/CS8	RS, Russian Maritime Register of Shipping

Note: Except for the CCS certificate, please consult the engineer for others.

Lithium battery	/LD	General requirements for low copper and zinc in the lithium battery industry
High-accuracy	/HAC	High-accuracy calibration according to the user's specified range Contract specifies: Range of use (within sensor's limit), LRL - URL, display unit, accuracy*
Language	/LE	English nameplate, operation manual, product certificate, etc.
Delivery service	/XM	Provide customer requested content according to project delivery standards
Extended warranty period	/Y3	3-year warranty
	/Y5	5-year warranty

***Note:** The specifications required for these options should be specified in the contract.

Example: MDM7000-LP-1HP1L-26-HF-2B1614AKU3S-LF-2B1614AKU3S/G1- 【CAL: 0-0.4bar】

|| Order Guide ||

MDM7000-LP — □□□□□ — □ — HE — □□□□□□ — LF — □□□□□□

Body

Remote Fixed Flange Insertion Sleeve
+Remote Fixed Flange Diaphragm

Item	Code	Description				
MDM7000-LP	—	Monocrystalline Silicon Differential Pressure Transmitter with Diaphragm Seals (Remote Fixed Flange Insertion Sleeve + Remote Fixed Flange)				
Application of hazardous area						
	1	China, Flameproof certificate, No.CE23.6650 Ex db IIC T6 Gb, GB/T3836.1-2021, GB/T3836.2-2021				
	2	China, Intrinsically safe certificate, No.CE23.7688X Ex ia IIC T4 Ga, GB/T3836.1-2021, GB/T3836.4-2021				
	3	China, Dust explosion-proof certificate, GYB24.1215X Ex tb III C T85°C Db, GB/T3836.1-2021, GB/T 3836.31-2021				
	4	China, Flameproof certificate, Intrinsically safe certificate				
	A	CSA, Flameproof certificate				
	B	CSA, Intrinsically safe certificate				
	C	CSA, Flameproof certificate, Intrinsically safe certificate				
	E	ATEX, Flameproof certificate				
	F	ATEX, Intrinsically safe certificate				
	G	ATEX, Flameproof certificate, Intrinsically safe certificate				
	J	IECEX, Flameproof certificate	 			
	K	IECEX, Intrinsically safe certificate				
	L	IECEX, Flameproof certificate, Intrinsically safe certificate				
	0	Non-hazardous area				
	T	Other certificate				
Output signal	H	4mA~20mA DC, HART				
Case	S	Stainless steel case with two outlet ports (F) M20×1.5				
	U	Stainless steel case with two outlet ports (F) 1/2NPT				
	P	Aluminum alloy case with two outlet ports (F) M20×1.5				
	N	Aluminum alloy case with two outlet ports (F) 1/2NPT				
Note: Please pay attention to the item of lithium battery (Code: LD)						
Waterproof/explosion-proof connector						
		Specification	Material	Applicable wire diameter	IP rating	
	1	M20×1.5 waterproof connector, with plug	PVC	6mm~8mm	IP67	
	2	Non-flameproof adapter (F) M20×1.5, with plug	316 SS	6mm~8mm	IP67	
	3	Flameproof adapter (F) 1/2NPT, with plug	316 SS	6mm~8mm	IP67	
	4	Flameproof adapter (F) M20×1.5, with plug	316 SS	6mm~8mm	IP67	
	5	Flameproof adapter (F) G1/2, with plug	316 SS	6mm~8mm	IP67	
Note: Flameproof configuration is applicable to PCEC/ATEX/IECEX standards. Flameproof adapter with CCC certificate. Please contact the engineer if double sealing is required.						
Display	N	Without LCD display				
	L	Display module, -20°C ~70°C				
Sensor module range						
		Nominal range	Minimum range	Lower (LRL)	Upper (URL)	
	2	0.4bar	0.1bar	-0.4bar	0.4bar	
	3	2.5bar	0.25bar	-2.5bar	2.5bar	
Clamp flange fastener	6	Bolts, nuts and other assemblies, 316 SS				

Diaphragm connection position	H	Differential pressure transmitter high pressure side		
Diaphragm seal system code	E	Remote fixed flange insertion sleeve		
Flange standard	2	HG/T-20592		
	1	EN1092-1		
	5	HG/T-20615		
	6	ANSI/ASME B16.5		
Flange diameter			Applicable standard	
	B	DN50	HG/T-20592, EN1092-1	
	C	DN80	HG/T-20592, EN1092-1	
	D	DN100	HG/T-20592, EN1092-1	
	2	2inch	HG/T-20615, ANSI/ASME B16.5	
	3	3inch	HG/T-20615, ANSI/ASME B16.5	
	4	4inch	HG/T-20615, ANSI/ASME B16.5	
Pressure class			Applicable standard	Applicable flange diameter
	1	PN10/PN16	HG/T-20592, EN1092-1	DN50, DN80, DN100
	2	PN25/PN40	HG/T-20592, EN1092-1	DN50, DN80, DN100
	3	PN63	HG/T-20592, EN1092-1	DN50, DN80
	4	PN100	HG/T-20592, EN1092-1	DN50, DN80
	A	Class 150	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	B	Class 300	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	C	Class 600	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch
Note: The maximum static pressure or overload depends on the flange pressure class				
Flange material	6	316 SS		
Flange sealing surface	1	RF Raised surface		
	A	FM Concave surface		
	B	M Convex surface		
	C	RJ Annular connection surface		
Note: For details about FM concave, M convex, RJ annular connection surface, please consult the engineer				
Insertion sleeve diameter			Applicable flange diameter	
	4	46mm	DN50, 2inch	
	6	66mm	DN80, 3inch	
	7	77mm	DN100, 4inch	
Insertion sleeve length	A	50mm		
	B	100mm		
	C	150mm		
	D	200mm		
Insertion sleeve material	6	316 SS		
Wetted parts material		Please see the material list of wetted parts for details		
		Blind	Measuring diaphragm	
	6A	316 SS	316L	
	6B	316 SS	Hastelloy C-276	
	6C	316 SS	Tantalum	
	6D	316 SS	Titanium	
	6E	316 SS	Monel	

Capillary connection location	K	Rear connection					
Capillary type	U	3.5mm OD (or 1ss/8 inch), armored 316L SS, PVC gray sheath					
	L	3.5mm OD (or 1/8 inch), armored 316L SS, stainless steel bellows sheath					
Capillary length		Insertion sleeve diameter	Adaptable measuring diaphragm				
			6A-316L	6B-HastelloyC-276	6C-Tantalum	6D-Titanium	6E-Monel
1	1m	S-46mm					
		M-66mm					
		L-77mm					
2	2m	S-46mm					
		M-66mm					
		L-77mm					
3	3m	S-46mm					
		M-66mm					
		L-77mm					
4	4m	S-46mm			x	x	x
		M-66mm					
		L-77mm					
5	5m	S-47mm			x	x	x
		M-66mm					
		L-77mm					
6	6m	M-66mm					
		L-77mm					
7	7m	M-66mm					
		L-77mm					
8	8m	M-66mm					
		L-77mm					
9	9m	M-66mm					
		L-77mm					
A	10m	M-66mm					
		L-77mm					

Note: "x" means unavailable; the part beyond the length will be selected according to the next level of meters.

High pressure side fill oil	S	Normal temperature silicone oil (Medium temperature : -40°C ~205°C , diaphragm ambient environment: -40°C ~85°C)
	D	Inert oil (Medium temperature: -45°C ~160°C ,diaphragm ambient environment:-40°C ~85°C)
	H	High temperature silicone oil (Medium temperature: 0°C ~315°C , diaphragm ambient environment: 0°C ~85°C)
Diaphragm connection position	L	Differential pressure transmitter low pressure side
Diaphragm seal system code	F	Remote fixed flange
Flange standard	2	HG/T-20592
	1	EN1092-1
	5	HG/T-20615
	6	ANSI/ASME B16.5

Flange diameter			Applicable standard
B	DN50		HG/T-20592, EN1092-1
C	DN80		HG/T-20592, EN1092-1
D	DN100		HG/T-20592, EN1092-1
2	2inch		HG/T-20615, ANSI/ASME B16.5
3	3inch		HG/T-20615, ANSI/ASME B16.5
4	4inch		HG/T-20615, ANSI/ASME B16.5

Pressure class			Applicable standard	Applicable flange diameter
1	PN10/PN16		HG/T-20592, EN1092-1	DN50, DN80, DN100
2	PN25/PN40		HG/T-20592, EN1092-1	DN50, DN80, DN100
3	PN63		HG/T-20592, EN1092-1	DN50, DN80
4	PN100		HG/T-20592, EN1092-1	DN50, DN80
A	Class 150		HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
B	Class 300		HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
C	Class 600		HG/T-20615, ANSI/ASME B16.5	2inch, 3inch

Note: The maximum static pressure or overload depends on the flange pressure class

Flange material	6	316 SS
Flange sealing surface	1	RF Raised surface
	A	FM Concave surface
	B	M Convex surface
	C	RJ Annular connection surface

Note: For details about FM concave, M convex, RJ annular connection surface, please consult the engineer

Wetted parts material	Please see the material list of wetted parts for details	
	Blind	Measuring diaphragm
6A	316 SS	316L
6B	316 SS	Hastelloy C-276
6C	316 SS	Tantalum
6D	316 SS	Titanium
6E	316 SS	Monel

Capillary connection location	K	Rear connection
Capillary type	U	3.5mm OD (or 1/8 inch), armored 316L SS, PVC gray sheath
	L	3.5mm OD (or 1/8 inch), armored 316L SS, stainless steel bellows sheath

Capillary length	Applicable flange diameter		
	DN50/2inch	DN80/3inch	DN100/4inch
1	1m		
2	2m		
3	3m		
4	4m		
5	5m		
6	6m	×	
7	7m	×	
8	8m	×	
9	9m	×	
A	10m	×	

Note: "×" means unavailable; the part beyond the length will be selected according to the next level of meters.

Low pressure side fill oil	S	Normal temperature silicone oil (Medium temperature : -40°C ~205°C , diaphragm ambient environment: -40°C ~85°C)
	D	Inert oil (Medium temperature: -45°C ~160°C ,diaphragm ambient environment:-40°C ~85°C)
	H	High temperature silicone oil (Medium temperature: 0°C ~315°C , diaphragm ambient environment: 0°C ~85°C)
Factory calibration range	CAL	Provides Micro Sensor standard verification report according to the range, and the default linear output Contract specifies: LRL - URL, display unit*
Options		Description (Detailed specifications as following, multiple options or null)
High vacuum high temperature	/V	High vacuum and high temperature process diaphragm (if this option is selected, the accuracy will be affected and can only up to 0.2%)
Mounting bracket	/G1	Bent bracket, 316 SS
Verification report	/Q1	Provide the Micro Sensor verification data according to user requirements Contract specifies: LRL - URL, display unit*
Note: Standard format follows the Micro Sensor's specifications. Select this option and provide the template if the customer specifies a format		
Damping time setting	/ST	Adjustable range 0s~100s, default 0s Contract specifies: Damping time*
Fault alarm setting	/WH	High alarm current value, 20.8mA
	/WL	Low alarm current value, 3.8mA, default
	/WS	Other saturation current values, specified within the range of 3.6mA~3.8mA or 20mA~22mA Contract specifies: saturation current values *
Product certificate	/QE	Standard format follows the Micro Sensor's specifications. Select this option and provide the template if the customer specifies a format
Identification plate	/PT	Product is shipped with an identification plate Contract specifies: Identification number, not exceeding 16 characters
Leakage test report	/QD4	PN10/PN16 (class150) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD5	PN25/PN40 (class300) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD6	PN63, Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD7	PN100 (class600) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
Note: The test pressure is the same as the flange pressure class		
HART configuration	/H5	HART5 configuration
Diaphragm with gold plated	/J3	Single diaphragm on high pressure side (5μ)
	/J4	Double diaphragms on high and low pressure sides (5μ)
Diaphragm spraying	/T3	High pressure side single insertion sleeve
	/T4	High pressure side single insertion sleeve and low pressure side single flange
Diaphragm sticking	/PFA	The diaphragm is stuck with PFA film, applicable to non-vacuum situations (pressure ≥ 0)
Oil-free treatment	/CL1	Degreasing and cleaning treatment of the wetted parts
Note: Please check the fill oil. Determine whether the inert filling oil is required (code: D).		



Certificates	/CS1	CCS, China Classification Society, TJ23PTB00014	
	/CS2	DNV, Det Norske Veritas	
	/CS3	BV, Bureau Veritas	
	/CS4	ABS, American Bureau of Shipping	
	/CS5	LR, Lloyd's Register of Shipping	
	/CS6	KR, Korean Register of Shipping	
	/CS7	NK, Nippon Kaiji Kyokai	
	/CS8	RS, Russian Maritime Register of Shipping	

Note: Except for the CCS certificate, please consult the engineer for others.

Lithium battery	/LD	General requirements for low copper and zinc in the lithium battery industry
High-accuracy	/HAC	High-accuracy calibration according to the user's specified range Contract specifies: Range of use (within sensor's limit), LRL - URL, display unit, accuracy*
Language	/LE	English nameplate, operation manual, product certificate, etc.
Delivery service	/XM	Provide customer requested content according to project delivery standards
Extended warranty period	/Y3	3-year warranty
	/Y5	5-year warranty

***Note:** The specifications required for these options should be specified in the contract.


Example: MDM7000-LP-1HP1L-2A1S1-HF-2B1614AKU3S/D1- 【CAL: 0-0.4bar】

|| Order Guide ||

MDM7000-LP — □□□□□ — □ — HE — □□□□□□ — LE — □□□□□□

Body

Remote Fixed Flange Insertion Sleeve
+Remote Fixed Flange Insertion Sleeve Diaphragm

Item	Code	Description	
MDM7000-LP	—	Monocrystalline Silicon Differential Pressure Transmitter with Diaphragm Seals (Remote Fixed Flange Insertion Sleeve+Remote Fixed Flange Insertion Sleeve)	
—			
Application of hazardous area			
	1	China, Flameproof certificate, No.CE23.6650 Ex db IIC T6 Gb, GB/T3836.1-2021, GB/T3836.2-2021	
	2	China, Intrinsically safe certificate, No.CE23.7688X Ex ia IIC T4 Ga, GB/T3836.1-2021, GB/T3836.4-2021	
	3	China, Dust explosion-proof certificate, GYB24.1215X Ex tb III C T85°C Db, GB/T3836.1-2021, GB/T 3836.31-2021	
	4	China, Flameproof certificate, Intrinsically safe certificate	
	A	CSA, Flameproof certificate	
	B	CSA, Intrinsically safe certificate	
	C	CSA, Flameproof certificate, Intrinsically safe certificate	
	E	ATEX, Flameproof certificate	
	F	ATEX, Intrinsically safe certificate	
	G	ATEX, Flameproof certificate, Intrinsically safe certificate	
	J	IECEX, Flameproof certificate	 
	K	IECEX, Intrinsically safe certificate	
	L	IECEX, Flameproof certificate, Intrinsically safe certificate	
	0	Non-hazardous area	
	T	Other certificate	
Output signal	H	4mA~20mA DC, HART	
Case	S	Stainless steel case with two outlet ports (F) M20×1.5	
	U	Stainless steel case with two outlet ports (F) 1/2NPT	
	P	Aluminum alloy case with two outlet ports (F) M20×1.5	
	N	Aluminum alloy case with two outlet ports (F) 1/2NPT	
Note: Please pay attention to the item of lithium battery (Code: LD)			
Waterproof/explosion-proof connector			
		Specification	Material
	1	M20×1.5 waterproof connector, with plug	PVC
	2	Non-flameproof adapter (F) M20×1.5, with plug	316 SS
	3	Flameproof adapter (F) 1/2NPT, with plug	316 SS
	4	Flameproof adapter (F) M20×1.5, with plug	316 SS
	5	Flameproof adapter (F) G1/2, with plug	316 SS
			Applicable wire diameter
			IP rating
			
Note: Flameproof configuration is applicable to PCEC/ATEX/IECEX standards. Flameproof adapter with CCC certificate.Please contact the engineer if double sealing is required.			
Display	N	Without LCD display	
	L	Display module, -20°C ~70°C	
—			
Sensor module range			
		Nominal range	Minimum range
		Lower (LRL)	Upper (URL)
	2	0.4bar	0.1bar
			-0.4bar
	3	2.5bar	0.25bar
			-2.5bar
Clamp flange fastener	6	Bolts, nuts and other assemblies, 316 SS	

Diaphragm connection position	H	Differential pressure transmitter high pressure side		
Diaphragm seal system code	E	Remote fixed flange insertion sleeve		
Flange standard	2	HG/T-20592		
	1	EN1092-1		
	5	HG/T-20615		
	6	ANSI/ASME B16.5		
Flange diameter			Applicable standard	
	B	DN50	HG/T-20592, EN1092-1	
	C	DN80	HG/T-20592, EN1092-1	
	D	DN100	HG/T-20592, EN1092-1	
	2	2inch	HG/T-20615, ANSI/ASME B16.5	
	3	3inch	HG/T-20615, ANSI/ASME B16.5	
	4	4inch	HG/T-20615, ANSI/ASME B16.5	
Pressure class			Applicable standard	Applicable flange diameter
	1	PN10/PN16	HG/T-20592, EN1092-1	DN50, DN80, DN100
	2	PN25/PN40	HG/T-20592, EN1092-1	DN50, DN80, DN100
	3	PN63	HG/T-20592, EN1092-1	DN50, DN80
	4	PN100	HG/T-20592, EN1092-1	DN50, DN80
	A	Class 150	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	B	Class 300	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	C	Class 600	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch
Note: The maximum static pressure or overload depends on the flange pressure class				
Flange material	6	316 SS		
Flange sealing surface	1	RF Raised surface		
	A	FM Concave surface		
	B	M Convex surface		
	C	RJ Annular connection surface		
Note: For details about FM concave, M convex, RJ annular connection surface, please consult the engineer				
Insertion sleeve diameter			Applicable flange diameter	
	4	46mm	DN50, 2inch	
	6	66mm	DN80, 3inch	
	7	77mm	DN100, 4inch	
Insertion sleeve length	A	50mm		
	B	100mm		
	C	150mm		
	D	200mm		
Insertion sleeve material	6	316 SS		
Wetted parts material		Please see the material list of wetted parts for details		
		Blind	Measuring diaphragm	
	6A	316 SS	316L	
	6B	316 SS	Hastelloy C-276	
	6C	316 SS	Tantalum	
	6D	316 SS	Titanium	
	6E	316 SS	Monel	

Capillary connection location	K	Rear connection					
Capillary type	U	3.5mm OD (or 1/8 inch), armored 316L SS, PVC gray sheath					
	L	3.5mm OD (or 1/8 inch), armored 316L SS, stainless steel bellows sheath					
Capillary length		Insertion sleeve diameter	Adaptable measuring diaphragm				
			6A-316L	6B-HastelloyC-276	6C-Tantalum	6D-Titanium	6E-Monel
1	1m	S-46mm					
		M-66mm					
		L-77mm					
2	2m	S-46mm					
		M-66mm					
		L-77mm					
3	3m	S-46mm					
		M-66mm					
		L-77mm					
4	4m	S-46mm			×	×	×
		M-66mm					
		L-77mm					
5	5m	S-47mm			×	×	×
		M-66mm					
		L-77mm					
6	6m	M-66mm					
		L-77mm					
7	7m	M-66mm					
		L-77mm					
8	8m	M-66mm					
		L-77mm					
9	9m	M-66mm					
		L-77mm					
A	10m	M-66mm					
		L-77mm					
Note: "x" means unavailable; the part beyond the length will be selected according to the next level of meters.							
High pressure side fill oil	S	Normal temperature silicone oil (Medium temperature : -40℃ ~205℃ , diaphragm ambient environment: -40℃ ~85℃)					
	D	Inert oil (Medium temperature: -45℃ ~160℃ ,diaphragm ambient environment:-40℃ ~85℃)					
	H	High temperature silicone oil (Medium temperature: 0℃ ~315℃ , diaphragm ambient environment: 0℃ ~85℃)					
Diaphragm connection position	L	Differential pressure transmitter low pressure side					
Diaphragm seal system code	E	Remote fixed flange insertion sleeve					
Flange standard	2	HG/T-20592					
	1	EN1092-1					
	5	HG/T-20615					
	6	ANSI/ASME B16.5					

Flange diameter			Applicable standard	
	B	DN50	HG/T-20592, EN1092-1	
	C	DN80	HG/T-20592, EN1092-1	
	D	DN100	HG/T-20592, EN1092-1	
	2	2inch	HG/T-20615, ANSI/ASME B16.5	
	3	3inch	HG/T-20615, ANSI/ASME B16.5	
	4	4inch	HG/T-20615, ANSI/ASME B16.5	
Pressure class			Applicable standard	Applicable flange diameter
	1	PN10/PN16	HG/T-20592, EN1092-1	DN50, DN80, DN100
	2	PN25/PN40	HG/T-20592, EN1092-1	DN50, DN80, DN100
	3	PN63	HG/T-20592, EN1092-1	DN50, DN80
	4	PN100	HG/T-20592, EN1092-1	DN50, DN80
	A	Class 150	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	B	Class 300	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	C	Class 600	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch
Note: The maximum static pressure or overload depends on the flange pressure class				
Flange material	6	316 SS		
Flange sealing surface	1	RF Raised surface		
	A	FM Concave surface		
	B	M Convex surface		
	C	RJ Annular connection surface		
Note: For details about FM concave, M convex, RJ annular connection surface, please consult the engineer				
Insertion sleeve diameter			Applicable flange diameter	
	4	46mm	DN50, 2inch	
	6	66mm	DN80, 3inch	
	7	77mm	DN100, 4inch	
Insertion sleeve length	A	50mm		
	B	100mm		
	C	150mm		
	D	200mm		
Insertion sleeve material	6	316 SS		
Wetted parts material		Please see the material list of wetted parts for details		
		Blind	Measuring diaphragm	
	6A	316 SS	316L	
	6B	316 SS	Hastelloy C-276	
	6C	316 SS	Tantalum	
	6D	316 SS	Titanium	
	6E	316 SS	Monel	
Capillary connection location	K	Rear connection		
Capillary type	U	3.5mm OD (or 1/8 inch), armored 316L SS, PVC gray sheath		
	L	3.5mm OD (or 1/8 inch), armored 316L SS, stainless steel bellows sheath		

Capillary length		Insertion sleeve diameter	Adaptable measuring diaphragm				
			6A-316L	6B-HastelloyC-276	6C-Tantalum	6D-Titanium	6E-Monel
1	1m	S-46mm					
		M-66mm					
		L-77mm					
2	2m	S-46mm					
		M-66mm					
		L-77mm					
3	3m	S-46mm					
		M-66mm					
		L-77mm					
4	4m	S-46mm			x	x	x
		M-66mm					
		L-77mm					
5	5m	S-47mm			x	x	x
		M-66mm					
		L-77mm					
6	6m	M-66mm					
		L-77mm					
7	7m	M-66mm					
		L-77mm					
8	8m	M-66mm					
		L-77mm					
9	9m	M-66mm					
		L-77mm					
A	10m	M-66mm					
		L-77mm					

Note: "x" means unavailable; the part beyond the length will be selected according to the next level of meters.

Low pressure side fill oil	S	Normal temperature silicone oil (Medium temperature : -40°C ~205°C , diaphragm ambient environment: -40°C ~85°C)
	D	Inert oil (Medium temperature: -45°C ~160°C ,diaphragm ambient environment:-40°C ~85°C)
	H	High temperature silicone oil (Medium temperature: 0°C ~315°C , diaphragm ambient environment: 0°C ~85°C)
Factory calibration range	CAL	Provides Micro Sensor standard verification report according to the range, and the default linear output Contract specifies: LRL - URL, display unit*
Options		Description (Detailed specifications as following, multiple options or null)
High vacuum high temperature	/V	High vacuum and high temperature process diaphragm (if this option is selected, the accuracy will be affected and can only up to 0.2%)
Mounting bracket	/G1	Bent bracket, 316 SS
Verification report	/Q1	Provide the Micro Sensor verification data according to user requirements Contract specifies: LRL - URL, display unit*
Note: Standard format follows the Micro Sensor's specifications. Select this option and provide the template if the customer specifies a format		
Damping time setting	/ST	Adjustable range 0~100s, default 0s Contract specifies: Damping time*
Fault alarm setting	/WH	High alarm current value, 20.8mA
	/WL	Low alarm current value, 3.8mA, default
	/WS	Other saturation current values, specified within the range of 3.6mA~3.8mA or 20mA~22mA Contract specifies: saturation current values *

Product certificate	/QE	Standard format follows the Micro Sensor's specifications. Select this option and provide the template if the customer specifies a format
Identification plate	/PT	Product is shipped with an identification plate Contract specifies: Identification number, not exceeding 16 characters
Leakage test report	/QD4	PN10/PN16 (class150) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD5	PN25/PN40 (class300) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD6	PN63, Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD7	PN100 (class600) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
Note: The test pressure is the same as the flange pressure class		
HART configuration	/H5	HART5 configuration
Diaphragm with gold plated	/J3	Single diaphragm on high pressure side (5μ)
	/J4	Double diaphragms on high and low pressure sides (5μ)
Diaphragm spraying	/T3	High pressure side single insertion sleeve
	/T5	High-low pressure side double insertion sleeve
Oil-free treatment	/CL1	Degreasing and cleaning treatment of the wetted parts
Note: Please check the fill oil. Determine whether the inert filling oil is required (code: D).		
Certificates	/CS1	CCS, China Classification Society, TJ23PTB00014
	/CS2	DNV, Det Norske Veritas
	/CS3	BV, Bureau Veritas
	/CS4	ABS, American Bureau of Shipping
	/CS5	LR, Lloyd's Register of Shipping
	/CS6	KR, Korean Register of Shipping
	/CS7	NK, Nippon Kaiji Kyokai
	/CS8	RS, Russian Maritime Register of Shipping
Note: Except for the CCS certificate, please consult the engineer for others.		
Lithium battery	/LD	General requirements for low copper and zinc in the lithium battery industry
High-accuracy	/HAC	High-accuracy calibration according to the user's specified range Contract specifies: Range of use (within sensor's limit), LRL - URL, display unit, accuracy*
Language	/LE	English nameplate, operation manual, product certificate, etc.
Delivery service	/XM	Provide customer requested content according to project delivery standards
Extended warranty period	/Y3	3-year warranty
	/Y5	5-year warranty

***Note:** The specifications required for these options should be specified in the contract.

Example: MDM7000-LP-1HP1L-26-HE-2B1614A6AKU3S-LE-2B1614A6AKU3S/G1- 【CAL: 0-0.4bar】

|| Order Guide ||

MDM7000-LP— □□□□□ — □ — HN — □□□□ — LF — □□□□□

Body

Side Mounted Movable Flange+Remote Fixed Flange Diaphragm

item	Code	Description
MDM7000-LT	—	Monocrystalline Silicon Differential Pressure Transmitter Side Mounted Remote Diaphragm Seals (Side Mounted Movable Flange + Remote Fixed Flange)

Application of hazardous area

1	China, Flameproof certificate, No.CE23.6650 Ex db IIC T6 Gb, GB/T3836.1-2021, GB/T3836.2-2021	
2	China, Intrinsically safe certificate, No.CE23.7688X Ex ia IIC T4 Ga, GB/T3836.1-2021, GB/T3836.4-2021	
3	China, Dust explosion-proof certificate, GYB24.1215X Ex tb III C T85°C Db, GB/T3836.1-2021, GB/T 3836.31-2021	
4	China, Flameproof certificate, Intrinsically safe certificate	
A	CSA, Flameproof certificate	
B	CSA, Intrinsically safe certificate	
C	CSA, Flameproof certificate, Intrinsically safe certificate	
E	ATEX, Flameproof certificate	
F	ATEX, Intrinsically safe certificate	
G	ATEX, Flameproof certificate, Intrinsically safe certificate	
J	IECEx, Flameproof certificate	
K	IECEx, Intrinsically safe certificate	
L	IECEx, Flameproof certificate, Intrinsically safe certificate	
O	Non-hazardous area	
T	Other certificate	

Output signal	H	4mA~20mA DC, HART	
Case	S	Stainless steel case with two outlet ports (F) M20×1.5	
	U	Stainless steel case with two outlet ports (F) 1/2NPT	
	P	Aluminum alloy case with two outlet ports (F) M20×1.5	
	N	Aluminum alloy case with two outlet ports (F) 1/2NPT	

Note: Please pay attention to the item of lithium battery (Code: LD)

Waterproof/explosion-proof connector

	Specification	Material	Applicable wire diameter	IP rating	
1	M20×1.5 waterproof connector, with plug	PVC	6mm~8mm	IP67	
2	Non-flameproof adapter (F) M20×1.5, with plug	316 SS	6mm~8mm	IP67	
3	Flameproof adapter (F) 1/2NPT, with plug	316 SS	6mm~8mm	IP67	
4	Flameproof adapter (F) M20×1.5, with plug	316 SS	6mm~8mm	IP67	
5	Flameproof adapter (F) G1/2, with plug	316 SS	6mm~8mm	IP67	

Note: Flameproof configuration is applicable to PCEC/ATEX/IECEx standards. Flameproof adapter with CCC certificate. Please contact the engineer if double sealing is required.

Display	N	Without LCD display	
	L	Display module, -20°C ~70°C	

Sensor module range

	Nominal range	Minimum range	Lower (LRL)	Upper (URL)
2	0.4bar	0.1bar	-0.4bar	0.4bar
3	2.5bar	0.25bar	-2.5bar	2.5bar

Clamp flange fastener	6	Bolts, nuts and other assemblies, 316 SS
-----------------------	---	--

Diaphragm connection position	H	Differential pressure transmitter high pressure side		
Diaphragm seal system code	N	Side mounted movable flange insertion sleeve		
Flange standard	2	HG/T-20592		
	1	EN1092-1		
	5	HG/T-20615		
	6	ANSI/ASME B16.5		
Flange diameter			Applicable standard	
	B	DN50	HG/T-20592, EN1092-1	
	C	DN80	HG/T-20592, EN1092-1	
	D	DN100	HG/T-20592, EN1092-1	
	2	2inch	HG/T-20615, ANSI/ASME B16.5	
	3	3inch	HG/T-20615, ANSI/ASME B16.5	
	4	4inch	HG/T-20615, ANSI/ASME B16.5	
Pressure class			Applicable standard	Applicable flange diameter
	1	PN10/PN16	HG/T-20592, EN1092-1	DN50, DN80, DN100
	2	PN25/PN40	HG/T-20592, EN1092-1	DN50, DN80, DN100
	3	PN63	HG/T-20592, EN1092-1	DN50, DN80
	4	PN100	HG/T-20592, EN1092-1	DN50, DN80
	A	Class 150	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	B	Class 300	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	C	Class 600	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch
Note: The maximum static pressure or overload depends on the flange pressure class				
Flange material	6	316 SS		
Blind sealing surface	1	RF Raised surface		
	A	FM Concave surface		
	B	M Convex surface		
	C	RJ Annular connection surface		
Note: For details about FM concave, M convex, RJ annular connection surface, please consult the engineer				
Wetted parts material		Please see the material list of wetted parts for details		
		Blind	Measuring diaphragm	
	6A	316 SS	316L	
	6B	316 SS	Hastelloy C-276	
	6C	316 SS	Tantalum	
	6D	316 SS	Titanium	
	6E	316 SS	Monel	
High pressure side fill oil	S	Normal temperature silicone oil (Medium temperature : -40°C ~205°C ,diaphragm ambient environment: -40°C ~85°C)		
	D	Inert oil (Medium temperature :-45°C ~160°C ,diaphragm ambient environment:-40°C ~85°C)		
	H	High temperature silicone oil (Medium temperature:0°C ~315°C ,diaphragm ambient environment:0°C ~85°C)		
Diaphragm connection position	L	Differential pressure transmitter low pressure side		
Diaphragm seal system code	F	Remote fixed flange		

Flange standard	2	HG/T-20592			
	1	EN1092-1			
	5	HG/T-20615			
	6	ANSI/ASME B16.5			
Flange diameter			Applicable standard		
	B	DN50	HG/T-20592, EN1092-1		
	C	DN80	HG/T-20592, EN1092-1		
	D	DN100	HG/T-20592, EN1092-1		
	2	2inch	HG/T-20615, ANSI/ASME B16.5		
	3	3inch	HG/T-20615, ANSI/ASME B16.5		
	4	4inch	HG/T-20615, ANSI/ASME B16.5		
Pressure class			Applicable standard	Applicable flange diameter	
	1	PN10/PN16	HG/T-20592, EN1092-1	DN50, DN80, DN100	
	2	PN25/PN40	HG/T-20592, EN1092-1	DN50, DN80, DN100	
	3	PN63	HG/T-20592, EN1092-1	DN50, DN80	
	4	PN100	HG/T-20592, EN1092-1	DN50, DN80	
	A	Class 150	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch	
	B	Class 300	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch	
	C	Class 600	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch	
Note: The maximum static pressure or overload depends on the flange pressure class					
Flange material	6	316 SS			
Flange sealing surface	1	RF Raised surface			
	A	FM Concave surface			
	B	M Convex surface			
	C	RJ Annular connection surface			
Note: For details about FM concave, M convex, RJ annular connection surface, please consult the engineer					
Insertion sleeve material	6	316 SS			
Wetted parts material		Please see the material list of wetted parts for details			
		Blind	Measuring diaphragm		
	6A	316 SS	316L		
	6B	316 SS	Hastelloy C-276		
	6C	316 SS	Tantalum		
	6D	316 SS	Titanium		
	6E	316 SS	Monel		
Capillary connection location	K	Rear connection			
Capillary type	U	3.5mm OD (or 1/8 inch), armored 316L SS, PVC gray sheath			
	L	3.5mm OD (or 1/8 inch), armored 316L SS, stainless steel bellows sheath			
Capillary length		Applicable flange diameter			
			DN50/2inch	DN80/3inch	DN100/4inch
	1	1m			
	2	2m			
	3	3m			
	4	4m			

5	5m		
6	6m	x	
7	7m	x	
8	8m	x	
9	9m	x	
A	10m	x	

Note: "x" means unavailable; the part beyond the length will be selected according to the next level of meters.

Low pressure side fill oil	S	Normal temperature silicone oil (Medium temperature : -40°C ~205°C , diaphragm ambient environment: -40°C ~85°C)
	D	Inert oil (Medium temperature: -45°C ~160°C ,diaphragm ambient environment:-40°C ~85°C)
	H	High temperature silicone oil (Medium temperature: 0°C ~315°C , diaphragm ambient environment: 0°C ~85°C)
Factory calibration range	CAL	Provides Micro Sensor standard verification report according to the range, and the default linear output Contract specifies: LRL - URL, display unit*
Options		Description (Detailed specifications as following, multiple options or null)
High vacuum high temperature	/V	High vacuum and high temperature process diaphragm (if this option is selected, the accuracy will be affected and can only up to 0.2%)
Verification report	/Q1	Provide the Micro Sensor verification data according to user requirements Contract specifies: LRL - URL, display unit*

Note: Standard format follows the Micro Sensor's specifications. Select this option and provide the template if the customer specifies a format

Damping time setting	/ST	Adjustable range 0s~100s, default 0s Contract specifies: Damping time*
Fault alarm setting	/WH	High alarm current value, 20.8mA
	/WL	Low alarm current value, 3.8mA, default
	/WS	Other saturation current values, specified within the range of 3.6mA~3.8mA or 20mA~22mA Contract specifies: saturation current values *
Product certificate	/QE	Standard format follows the Micro Sensor's specifications. Select this option and provide the template if the customer specifies a format
Identification plate	/PT	Product is shipped with an identification plate Contract specifies: Identification number, not exceeding 16 characters
Leakage test report	/QD4	PN10/PN16 (class150) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD5	PN25/PN40 (class300) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD6	PN63, Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD7	PN100 (class600) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report

Note: The test pressure is the same as the flange pressure class

HART configuration	/H5	HART5 configuration
Diaphragm with gold plated	/J3	Single diaphragm on high pressure side (5μ)
	/J4	Double diaphragms on high and low pressure sides (5μ)
Diaphragm spraying	/T1	High pressure side single flange
	/T2	High-low pressure side double flange
Diaphragm sticking	/PFA	The diaphragm is stuck with PFA film, applicable to non-vacuum situations (pressure ≥ 0)
Oil-free treatment	/CL1	Degreasing and cleaning treatment of the wetted parts



Note: Please check the fill oil. Determine whether the inert filling oil is required (code: D).

Certificates	/CS1	CCS, China Classification Society, TJ23PTB00014	
	/CS2	DNV, Det Norske Veritas	
	/CS3	BV, Bureau Veritas	
	/CS4	ABS, American Bureau of Shipping	
	/CS5	LR, Lloyd's Register of Shipping	
	/CS6	KR, Korean Register of Shipping	
	/CS7	NK, Nippon Kaiji Kyokai	
	/CS8	RS, Russian Maritime Register of Shipping	

Note: Except for the CCS certificate, please consult the engineer for others.

Lithium battery	/LD	General requirements for low copper and zinc in the lithium battery industry
High-accuracy	/HAC	High-accuracy calibration according to the user's specified range Contract specifies: Range of use (within sensor's limit), LRL - URL, display unit, accuracy*
Language	/LE	English nameplate, operation manual, product certificate, etc.
Delivery service	/XM	Provide customer requested content according to project delivery standards
Extended warranty period	/Y3	3-year warranty
	/Y5	5-year warranty

***Note:** The specifications required for these options should be specified in the contract.

Example: MDM7000-LP-1HP1L-2A1S1-HN-22B1616AS-LF-2B1614AKU3S/CS1- 【CAL: 0-0.4bar】

Order Guide

MDM7000-LP — ☐☐☐☐☐ — ☐ — **HM** — ☐☐☐☐☐☐☐ **LF** — ☐☐☐☐☐☐

Body

Side Mounted Movable Flange Insertion Sleeve+Remote Fixed Flange Diaphragm

Item	Code	Description				
MDM7000-LP	—	Monocrystalline Silicon Differential Pressure Transmitter Side Mounted Remote Diaphragm Seals (Side Mounted Movable Flange Insertion Sleeve + Remote Fixed Flange)				
Application of hazardous area						
	1	China, Flameproof certificate, No.CE23.6650 Ex db IIC T6 Gb, GB/T3836.1-2021, GB/T3836.2-2021				
	2	China, Intrinsically safe certificate, No.CE23.7688X Ex ia IIC T4 Ga, GB/T3836.1-2021, GB/T3836.4-2021				
	3	China, Dust explosion-proof certificate, GYB24.1215X Ex tb III C T85°C Db, GB/T3836.1-2021, GB/T 3836.31-2021				
	4	China, Flameproof certificate, Intrinsically safe certificate				
	A	CSA, Flameproof certificate				
	B	CSA, Intrinsically safe certificate				
	C	CSA, Flameproof certificate, Intrinsically safe certificate				
	E	ATEX, Flameproof certificate				
	F	ATEX, Intrinsically safe certificate				
	G	ATEX, Flameproof certificate, Intrinsically safe certificate				
	J	IECEX, Flameproof certificate	 			
	K	IECEX, Intrinsically safe certificate				
	L	IECEX, Flameproof certificate, Intrinsically safe certificate				
	0	Non-hazardous area				
	T	Other certificate				
Output signal	H	4mA~20mA DC, HART				
Case	S	Stainless steel case with two outlet ports (F) M20×1.5				
	U	Stainless steel case with two outlet ports (F) 1/2NPT				
	P	Aluminum alloy case with two outlet ports (F) M20×1.5				
	N	Aluminum alloy case with two outlet ports (F) 1/2NPT				
Note: Please pay attention to the item of lithium battery (Code: LD)						
Waterproof/explosion-proof connector						
		Specification	Material	Applicable wire diameter	IP rating	
	1	M20×1.5 waterproof connector, with plug	PVC	6mm~8mm	IP67	
	2	Non-flameproof adapter (F) M20×1.5, with plug	316 SS	6mm~8mm	IP67	
	3	Flameproof adapter (F) 1/2NPT, with plug	316 SS	6mm~8mm	IP67	
	4	Flameproof adapter (F) M20×1.5, with plug	316 SS	6mm~8mm	IP67	
	5	Flameproof adapter (F) G1/2, with plug	316 SS	6mm~8mm	IP67	
Note: Flameproof configuration is applicable to PCEC/ATEX/IECEX standards. Flameproof adapter with CCC certificate. Please contact the engineer if double sealing is required.						
Display	N	Without LCD display				
	L	Display module, -20°C ~70°C				
Sensor module range						
		Nominal range	Minimum range	Lower (LRL)	Upper (URL)	
	2	0.4bar	0.1bar	-0.4bar	0.4bar	
	3	2.5bar	0.25bar	-2.5bar	2.5bar	
Clamp flange fastener	6	Bolts, nuts and other assemblies, 316 SS				

Diaphragm connection position	H	Differential pressure transmitter high pressure side		
Diaphragm seal system code	M	Side mounted movable flange insertion sleeve		
Flange standard	2	HG/T-20592		
	1	EN1092-1		
	5	HG/T-20615		
	6	ANSI/ASME B16.5		
Flange diameter			Applicable standard	
	B	DN50	HG/T-20592, EN1092-1	
	C	DN80	HG/T-20592, EN1092-1	
	D	DN100	HG/T-20592, EN1092-1	
	2	2inch	HG/T-20615, ANSI/ASME B16.5	
	3	3inch	HG/T-20615, ANSI/ASME B16.5	
	4	4inch	HG/T-20615, ANSI/ASME B16.5	
Pressure class			Applicable standard	Applicable flange diameter
	1	PN10/PN16	HG/T-20592, EN1092-1	DN50, DN80, DN100
	2	PN25/PN40	HG/T-20592, EN1092-1	DN50, DN80, DN100
	3	PN63	HG/T-20592, EN1092-1	DN50, DN80
	4	PN100	HG/T-20592, EN1092-1	DN50, DN80
	A	Class 150	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	B	Class 300	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	C	Class 600	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch
Note: The maximum static pressure or overload depends on the flange pressure class				
Flange material	6	316 SS		
Blind sealing surface	1	RF Raised surface		
	A	FM Concave surface		
	B	M Convex surface		
	C	RJ Annular connection surface		
Note: For details about FM concave, M convex, RJ annular connection surface, please consult the engineer				
Insertion sleeve diameter			Applicable flange diameter	
	4	46mm	DN50, 2inch	
	6	66mm	DN80, 3inch	
	7	77mm	DN100, 4inch	
Insertion sleeve length	A	50mm		
	B	100mm		
	C	150mm		
	D	200mm		
Insertion sleeve material	6	316 SS		
Wetted parts material		Please see the material list of wetted parts for details		
		Blind	Measuring diaphragm	
	6A	316 SS	316L	
	6B	316 SS	Hastelloy C-276	
	6C	316 SS	Tantalum	
	6D	316 SS	Titanium	

High pressure side fill oil	S	Normal temperature silicone oil （Medium temperature：-40℃ ~205℃ ,diaphragm ambient environment：-40℃ ~85℃）		
	D	Inert oil （Medium temperature：-45℃ ~160℃ ,diaphragm ambient environment:-40℃ ~85℃）		
	H	High temperature silicone oil （Medium temperature:0℃ ~315℃ ,diaphragm ambient environment:0℃ ~85℃）		
Diaphragm connection position	L	Differential pressure transmitter low pressure side		
Diaphragm seal system code	F	Remote fixed flange		
Flange standard	2	HG/T-20592		
	1	EN1092-1		
	5	HG/T-20615		
	6	ANSI/ASME B16.5		
Flange diameter			Applicable standard	
	B	DN50	HG/T-20592, EN1092-1	
	C	DN80	HG/T-20592, EN1092-1	
	D	DN100	HG/T-20592, EN1092-1	
	2	2inch	HG/T-20615, ANSI/ASME B16.5	
	3	3inch	HG/T-20615, ANSI/ASME B16.5	
	4	4inch	HG/T-20615, ANSI/ASME B16.5	
Pressure class			Applicable standard	Applicable flange diameter
	1	PN10/PN16	HG/T-20592, EN1092-1	DN50, DN80, DN100
	2	PN25/PN40	HG/T-20592, EN1092-1	DN50, DN80, DN100
	3	PN63	HG/T-20592, EN1092-1	DN50, DN80
	4	PN100	HG/T-20592, EN1092-1	DN50, DN80
	A	Class 150	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	B	Class 300	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	C	Class 600	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch
Note: The maximum static pressure or overload depends on the flange pressure class				
Flange material	6	316 SS		
Flange sealing surface	1	RF Raised surface		
	A	FM Concave surface		
	B	M Convex surface		
	C	RJ Annular connection surface		
Note: For details about FM concave, M convex, RJ annular connection surface, please consult the engineer				
Wetted parts material		Please see the material list of wetted parts for details		
		Blind	Measuring diaphragm	
	6A	316 SS	316L	
	6B	316 SS	Hastelloy C-276	
	6C	316 SS	Tantalum	
	6D	316 SS	Titanium	
	6E	316 SS	Monel	
Capillary connection location	K	Rear connection		
Capillary type	U	3.5mm OD (or 1/8 inch), armored 316L SS, PVC gray sheath		
	L	3.5mm OD (or 1/8 inch), armored 316L SS, stainless steel bellows sheath		

Capillary length		Applicable flange diameter		
		DN50/2inch	DN80/3inch	DN100/4inch
1	1m			
2	2m			
3	3m			
4	4m			
5	5m			
6	6m	x		
7	7m	x		
8	8m	x		
9	9m	x		
A	10m	x		

Note: "x" means unavailable; the part beyond the length will be selected according to the next level of meters.

Low pressure side fill oil	S	Normal temperature silicone oil (Medium temperature : -40°C ~205°C , diaphragm ambient environment: -40°C ~85°C)
	D	Inert oil (Medium temperature: -45°C ~160°C ,diaphragm ambient environment:-40°C ~85°C)
	H	High temperature silicone oil (Medium temperature: 0°C ~315°C , diaphragm ambient environment: 0°C ~85°C)

Factory calibration range	CAL	Provides Micro Sensor standard verification report according to the range, and the default linear output Contract specifies: LRL - URL, display unit*
---------------------------	-----	---

Options	Description (Detailed specifications as following, multiple options or null)	
---------	--	--

High vacuum high temperature	/V	High vacuum and high temperature process diaphragm (if this option is selected, the accuracy will be affected and can only up to 0.2%)
------------------------------	----	--

Verification report	/Q1	Provide the Micro Sensor verification data according to user requirements Contract specifies: LRL - URL, display unit*
---------------------	-----	--

Note: Standard format follows the Micro Sensor's specifications. Select this option and provide the template if the customer specifies a format

Damping time setting	/ST	Adjustable range 0s~100s, default 0s Contract specifies: Damping time*
----------------------	-----	--

Fault alarm setting	/WH	High alarm current value, 20.8mA
	/WL	Low alarm current value, 3.8mA, default
	/WS	Other saturation current values, specified within the range of 3.6mA~3.8mA or 20mA~22mA Contract specifies: saturation current values *

Product certificate	/QE	Standard format follows the Micro Sensor's specifications. Select this option and provide the template if the customer specifies a format
---------------------	-----	---

Identification plate	/PT	Product is shipped with an identification plate Contract specifies: Identification number, not exceeding 16 characters
----------------------	-----	--

Leakage test report	/QD4	PN10/PN16 (class150) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD5	PN25/PN40 (class300) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD6	PN63, Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD7	PN100 (class600) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report

Note: The test pressure is the same as the flange pressure class

HART configuration	/H5	HART5 configuration
--------------------	-----	---------------------

Diaphragm with gold plated	/J3	Single diaphragm on high pressure side (5μ)
	/J4	Double diaphragms on high and low pressure sides (5μ)



Diaphragm spraying	/T3	Single insertion sleeve on high pressure side
	/T4	Single insertion sleeve on high pressure side and single flange on low pressure side
Diaphragm sticking	/PFA	The diaphragm is stuck with PFA film, applicable to non-vacuum situations (pressure ≥ 0)
Note: Sticking is not available on the insertion sleeve		
Oil-free treatment	/CL1	Degreasing and cleaning treatment of the wetted parts
Note: Please check the fill oil. Determine whether the inert filling oil is required (code: D).		
Certificates	/CS1	CCS, China Classification Society, TJ23PTB00014
	/CS2	DNV, Det Norske Veritas
	/CS3	BV, Bureau Veritas
	/CS4	ABS, American Bureau of Shipping
	/CS5	LR, Lloyd's Register of Shipping
	/CS6	KR, Korean Register of Shipping
	/CS7	NK, Nippon Kaiji Kyokai
	/CS8	RS, Russian Maritime Register of Shipping
Note: Except for the CCS certificate, please consult the engineer for others.		
Lithium battery	/LD	General requirements for low copper and zinc in the lithium battery industry
High-accuracy	/HAC	High-accuracy calibration according to the user's specified range Contract specifies: Range of use (within sensor's limit), LRL - URL, display unit, accuracy*
Language	/LE	English nameplate, operation manual, product certificate, etc.
Delivery service	/XM	Provide customer requested content according to project delivery standards
Extended warranty period	/Y3	3-year warranty
	/Y5	5-year warranty

***Note:** The specifications required for these options should be specified in the contract.

Example: MDM7000-LP-1HP1L-21-HM-2B14614A66AS-LF-2B1614AKU3S/CS1- 【CAL: 0-0.4bar】



|| Order Guide ||

MDM7000-LP — ☐☐☐☐☐ — ☐ — HM — ☐☐☐☐☐☐ — LE ☐☐☐☐☐☐

Body

Side Mounted Movable Flange Insertion Sleeve +
Remote Fixed Flange Insertion Sleeve

Item	Code	Description				
MDM7000-LP	—	Monocrystalline Silicon Differential Pressure Transmitter Side Mounted Remote Diaphragm Seals (Side Mounted Movable Flange Insertion Sleeve + Remote Fixed Flange Insertion Sleeve)				
Application of hazardous area						
	1	China, Flameproof certificate, No.CE23.6650 Ex db IIC T6 Gb, GB/T3836.1-2021, GB/T3836.2-2021				
	2	China, Intrinsically safe certificate, No.CE23.7688X Ex ia IIC T4 Ga, GB/T3836.1-2021, GB/T3836.4-2021				
	3	China, Dust explosion-proof certificate, GYB24.1215X Ex tb III C T85°C Db, GB/T3836.1-2021, GB/T 3836.31-2021				
	4	China, Flameproof certificate, Intrinsically safe certificate				
	A	CSA, Flameproof certificate				
	B	CSA, Intrinsically safe certificate				
	C	CSA, Flameproof certificate, Intrinsically safe certificate				
	E	ATEX, Flameproof certificate				
	F	ATEX, Intrinsically safe certificate				
	G	ATEX, Flameproof certificate, Intrinsically safe certificate				
	J	IECEX, Flameproof certificate	 			
	K	IECEX, Intrinsically safe certificate				
	L	IECEX, Flameproof certificate, Intrinsically safe certificate				
	0	Non-hazardous area				
	T	Other certificate				
Output signal	H	4mA~20mA DC, HART				
Case	S	Stainless steel case with two outlet ports (F) M20×1.5				
	U	Stainless steel case with two outlet ports (F) 1/2NPT				
	P	Aluminum alloy case with two outlet ports (F) M20×1.5				
	N	Aluminum alloy case with two outlet ports (F) 1/2NPT				
Note: Please pay attention to the item of lithium battery (Code: LD)						
Waterproof/explosion-proof connector						
		Specification	Material	Applicable wire diameter	IP rating	
	1	M20×1.5 waterproof connector, with plug	PVC	6mm~8mm	IP67	
	2	Non-flameproof adapter (F) M20×1.5, with plug	316 SS	6mm~8mm	IP67	
	3	Flameproof adapter (F) 1/2NPT, with plug	316 SS	6mm~8mm	IP67	
	4	Flameproof adapter (F) M20×1.5, with plug	316 SS	6mm~8mm	IP67	
	5	Flameproof adapter (F) G1/2, with plug	316 SS	6mm~8mm	IP67	
Note: Flameproof configuration is applicable to PCEC/ATEX/IECEX standards. Flameproof adapter with CCC certificate. Please contact the engineer if double sealing is required.						
Display	N	Without LCD display				
	L	Display module, -20°C ~70°C				
Sensor module range						
		Nominal range	Minimum range	Lower (LRL)	Upper (URL)	
	2	0.4bar	0.1bar	-0.4bar	0.4bar	
	3	2.5bar	0.25bar	-2.5bar	2.5bar	
Clamp flange fastener	6	Bolts, nuts and other assemblies, 316 SS				

Diaphragm connection position	H	Differential pressure transmitter high pressure side		
Diaphragm system code	M	Side-mounted movable flange insertion sleeve		
Flange standard	2	HG/T-20592		
	1	EN1092-1		
	5	HG/T-20615		
	6	ANSI/ASME B16.5		
Flange diameter			Applicable standard	
	B	DN50	HG/T-20592, EN1092-1	
	C	DN80	HG/T-20592, EN1092-1	
	D	DN100	HG/T-20592, EN1092-1	
	2	2inch	HG/T-20615, ANSI/ASME B16.5	
	3	3inch	HG/T-20615, ANSI/ASME B16.5	
	4	4inch	HG/T-20615, ANSI/ASME B16.5	
Pressure class			Applicable standard	Applicable flange diameter
	1	PN10/PN16	HG/T-20592, EN1092-1	DN50, DN80, DN100
	2	PN25/PN40	HG/T-20592, EN1092-1	DN50, DN80, DN100
	3	PN63	HG/T-20592, EN1092-1	DN50, DN80
	4	PN100	HG/T-20592, EN1092-1	DN50, DN80
	A	Class 150	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	B	Class 300	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch, 4inch
	C	Class 600	HG/T-20615, ANSI/ASME B16.5	2inch, 3inch
Note: The maximum static pressure or overload depends on the flange pressure class				
Flange material	6	316 SS		
Flange sealing surface	1	RF Raised surface		
	A	FM Concave surface		
	B	M Convex surface		
	C	RJ Annular connection surface		
Note: For details about FM concave, M convex, RJ annular connection surface, please consult the engineer				
Insertion sleeve diameter			Applicable flange diameter	
	4	46mm	DN50, 2inch	
	6	66mm	DN80, 3inch	
	7	77mm	DN100, 4inch	
Insertion sleeve length	A	50mm		
	B	100mm		
	C	150mm		
	D	200mm		
Insertion sleeve material	6	316 SS		
Wetted parts material		Please see the material list of wetted parts for details		
		Blind	Measuring diaphragm	
	6A	316 SS	316L	
	6B	316 SS	Hastelloy C-276	
	6C	316 SS	Tantalum	
	6D	316 SS	Titanium	
	6E	316 SS	Monel	

Wetted parts material		Please see the material list of wetted parts for details					
		Blind	Measuring diaphragm				
	6A	316 SS	316L				
	6B	316 SS	Hastelloy C-276				
	6C	316 SS	Tantalum				
	6D	316 SS	Titanium				
	6E	316 SS	Monel				
Capillary connection location	K	Rear connection					
Capillary type	U	3.5mm OD (or 1/8 inch), armored 316L SS, PVC gray sheath					
	L	3.5mm OD (or 1/8 inch), armored 316L SS, stainless steel bellows sheath					
Capillary length		Insertion sleeve diameter	Adaptable measuring diaphragm				
			6A-316L	6B-HastelloyC-276	6C-Tantalum	6D-Titanium	6E-Monel
1	1m	S-46mm					
		M-66mm					
		L-77mm					
2	2m	S-46mm					
		M-66mm					
		L-77mm					
3	3m	S-46mm					
		M-66mm					
		L-77mm					
4	4m	S-46mm			x	x	x
		M-66mm					
		L-77mm					
5	5m	S-47mm			x	x	x
		M-66mm					
		L-77mm					
6	6m	M-66mm					
		L-77mm					
7	7m	M-66mm					
		L-77mm					
8	8m	M-66mm					
		L-77mm					
9	9m	M-66mm					
		L-77mm					
A	10m	M-66mm					
		L-77mm					
Note: "x" means unavailable; the part beyond the length will be selected according to the next level of meters.							
Low pressure side fill oil	S	Normal temperature silicone oil (Medium temperature : -40°C ~205°C , diaphragm ambient environment: -40°C ~85°C)					
	D	Inert oil (Medium temperature: -45°C ~160°C ,diaphragm ambient environment:-40°C ~85°C)					
	H	High temperature silicone oil (Medium temperature: 0°C ~315°C , diaphragm ambient environment: 0°C ~85°C)					
Factory calibration range	CAL	Provides Micro Sensor standard verification report according to the range, and the default linear output Contract specifies: LRL - URL, displav unit*					

Options		Description (Detailed specifications as following, multiple options or null)
High vacuum high temperature	/V	High vacuum and high temperature process diaphragm (if this option is selected, the accuracy will be affected and can only up to 0.2%)
Verification report	/Q1	Provide the Micro Sensor verification data according to user requirements Contract specifies: LRL - URL, display unit*
Note: Standard format follows the Micro Sensor's specifications. Select this option and provide the template if the customer specifies a format		
Damping time setting	/ST	Adjustable range 0~100s, default 0s Contract specifies: Damping time*
Fault alarm setting	/WH	High alarm current value, 20.8mA
	/WL	Low alarm current value, 3.8mA, default
	/WS	Other saturation current values, specified within the range of 3.6mA~3.8mA or 20mA~22mA Contract specifies: saturation current values *
Product certificate	/QE	Standard format follows the Micro Sensor's specifications. Select this option and provide the template if the customer specifies a format
Identification plate	/PT	Product is shipped with an identification plate Contract specifies: Identification number, not exceeding 16 characters
Leakage test report	/QD4	PN10/PN16 (class150) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD5	PN25/PN40 (class300) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD6	PN63, Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
	/QD7	PN100 (class600) , Nitrogen (N2) or air, pressure holding for 10 minutes, provide Micro Sensor standard leakage test report
Note: The test pressure is the same as the flange pressure class		
HART configuration	/H5	HART5 configuration
Diaphragm with gold plated	/J3	Single diaphragm on high pressure side (5μ)
	/J4	Double diaphragms on high and low pressure sides (5μ)
Diaphragm spraying	/T3	High pressure side single insertion sleeve
	/T5	High-low pressure side double insertion sleeve
Oil-free treatment	/CL1	Degreasing and cleaning treatment of the wetted parts
Note: Please check the fill oil. Determine whether the inert filling oil is required (code: D).		
Certificates	/CS1	CCS, China Classification Society, TJ23PTB00014
	/CS2	DNV, Det Norske Veritas
	/CS3	BV, Bureau Veritas
	/CS4	ABS, American Bureau of Shipping
	/CS5	LR, Lloyd's Register of Shipping
	/CS6	KR, Korean Register of Shipping
	/CS7	NK, Nippon Kaiji Kyokai
	/CS8	RS, Russian Maritime Register of Shipping



Note: Except for the CCS certificate, please consult the engineer for others.

Lithium battery	/LD	General requirements for low copper and zinc in the lithium battery industry
High-accuracy	/HAC	High-accuracy calibration according to the user's specified range Contract specifies: Range of use (within sensor's limit), LRL - URL, display unit, accuracy*
Language	/LE	English nameplate, operation manual, product certificate, etc.
Delivery service	/XM	Provide customer requested content according to project delivery standards
Extended warranty period	/Y3	3-year warranty
	/Y5	5-year warranty

***Note:** The specifications required for these options should be specified in the contract.

Example: MDM7000-LP-1HP1L-21-HM-2B1614A6AKU3S-LE-2B1614A6AKU3S/CS1- 【CAL: 0-0.4bar】

Алматы (7273)495-231
Ангарск (3955)60-70-56
Архангельск (8182)63-90-72
Астрахань (8512)99-46-04
Барнаул (3852)73-04-60
Белгород (4722)40-23-64
Благовещенск (4162)22-76-07
Брянск (4832)59-03-52
Владивосток (423)249-28-31
Владикавказ (8672)28-90-48
Владимир (4922)49-43-18
Волгоград (844)278-03-48
Вологда (8172)26-41-59
Воронеж (473)204-51-73
Екатеринбург (343)384-55-89

Иваново (4932)77-34-06
Ижевск (3412)26-03-58
Иркутск (395)279-98-46
Казань (843)206-01-48
Калининград (4012)72-03-81
Калуга (4842)92-23-67
Кемерово (3842)65-04-62
Киров (8332)68-02-04
Коломна (4966)23-41-49
Кострома (4942)77-07-48
Краснодар (861)203-40-90
Красноярск (391)204-63-61
Курск (4712)77-13-04
Курган (3522)50-90-47
Липецк (4742)52-20-81

Магнитогорск (3519)55-03-13
Москва (495)268-04-70
Мурманск (8152)59-64-93
Набережные Челны (8552)20-53-41
Нижний Новгород (831)429-08-12
Новокузнецк (3843)20-46-81
Ноябрьск (3496)41-32-12
Новосибирск (383)227-86-73
Омск (3812)21-46-40
Орел (4862)44-53-42
Оренбург (3532)37-68-04
Пенза (8412)22-31-16
Петрозаводск (8142)55-98-37
Псков (8112)59-10-37
Пермь (342)205-81-47

Ростов-на-Дону (863)308-18-15
Рязань (4912)46-61-64
Самара (846)206-03-16
Санкт-Петербург (812)309-46-40
Саратов (845)249-38-78
Севастополь (8692)22-31-93
Саранск (8342)22-96-24
Симферополь (3652)67-13-56
Смоленск (4812)29-41-54
Сочи (862)225-72-31
Ставрополь (8652)20-65-13
Сургут (3462)77-98-35
Сыктывкар (8212)25-95-17
Тамбов (4752)50-40-97
Тверь (4822)63-31-35

Тольятти (8482)63-91-07
Томск (3822)98-41-53
Тула (4872)33-79-87
Тюмень (3452)66-21-18
Ульяновск (8422)24-23-59
Улан-Удэ (3012)59-97-51
Уфа (347)229-48-12
Хабаровск (4212)92-98-04
Чебоксары (8352)28-53-07
Челябинск (351)202-03-61
Череповец (8202)49-02-64
Чита (3022)38-34-83
Якутск (4112)23-90-97
Ярославль (4852)69-52-93

Россия +7(495)268-04-70

Казахстан +7(7172)727-132

Киргизия +996(312)96-26-47

<https://microsensor.nt-rt.ru/> || moj@nt-rt.ru